

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
29 March 2001 (29.03.2001)

PCT

(10) International Publication Number  
**WO 01/21102 A1**

(51) International Patent Classification<sup>7</sup>: A61F 2/06

(AU). YU, Weiyun; Apt. 59 #8, Birchgrove, New South Wales 2041 (AU).

(21) International Application Number: PCT/US00/16457

(74) Agents: GLUCK, Peter, J. et al.; Edwards Lifesciences LLC, One Baxter Way, Irvine, CA 92614 (US).

(22) International Filing Date: 15 June 2000 (15.06.2000)

(25) Filing Language: English

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW.

(26) Publication Language: English

(30) Priority Data:  
PQ 3027 23 September 1999 (23.09.1999) AU  
09/473,618 29 December 1999 (29.12.1999) US

(71) Applicants: EDWARDS LIFESCIENCES CORPORATION [US/US]; One Edwards Way, Irvine, CA 92614 (US). ENDOGAD RESEARCH PTY. LIMITED [AU/AU]; P.O. Box M88, Camperdown, New South Wales 2050 (AU).


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

(72) Inventors: DEHDASHTIAN, Mark; 1696 Palau Place, Costa Mesa, CA 92626 (US). WHITE, Geoffrey, H.; 22 Nicholson Street, East Balmain, New South Wales 2041

Published:  
— With international search report.

[Continued on next page]

(54) Title: DOUBLE LAYER INTRALUMINAL GRAFT

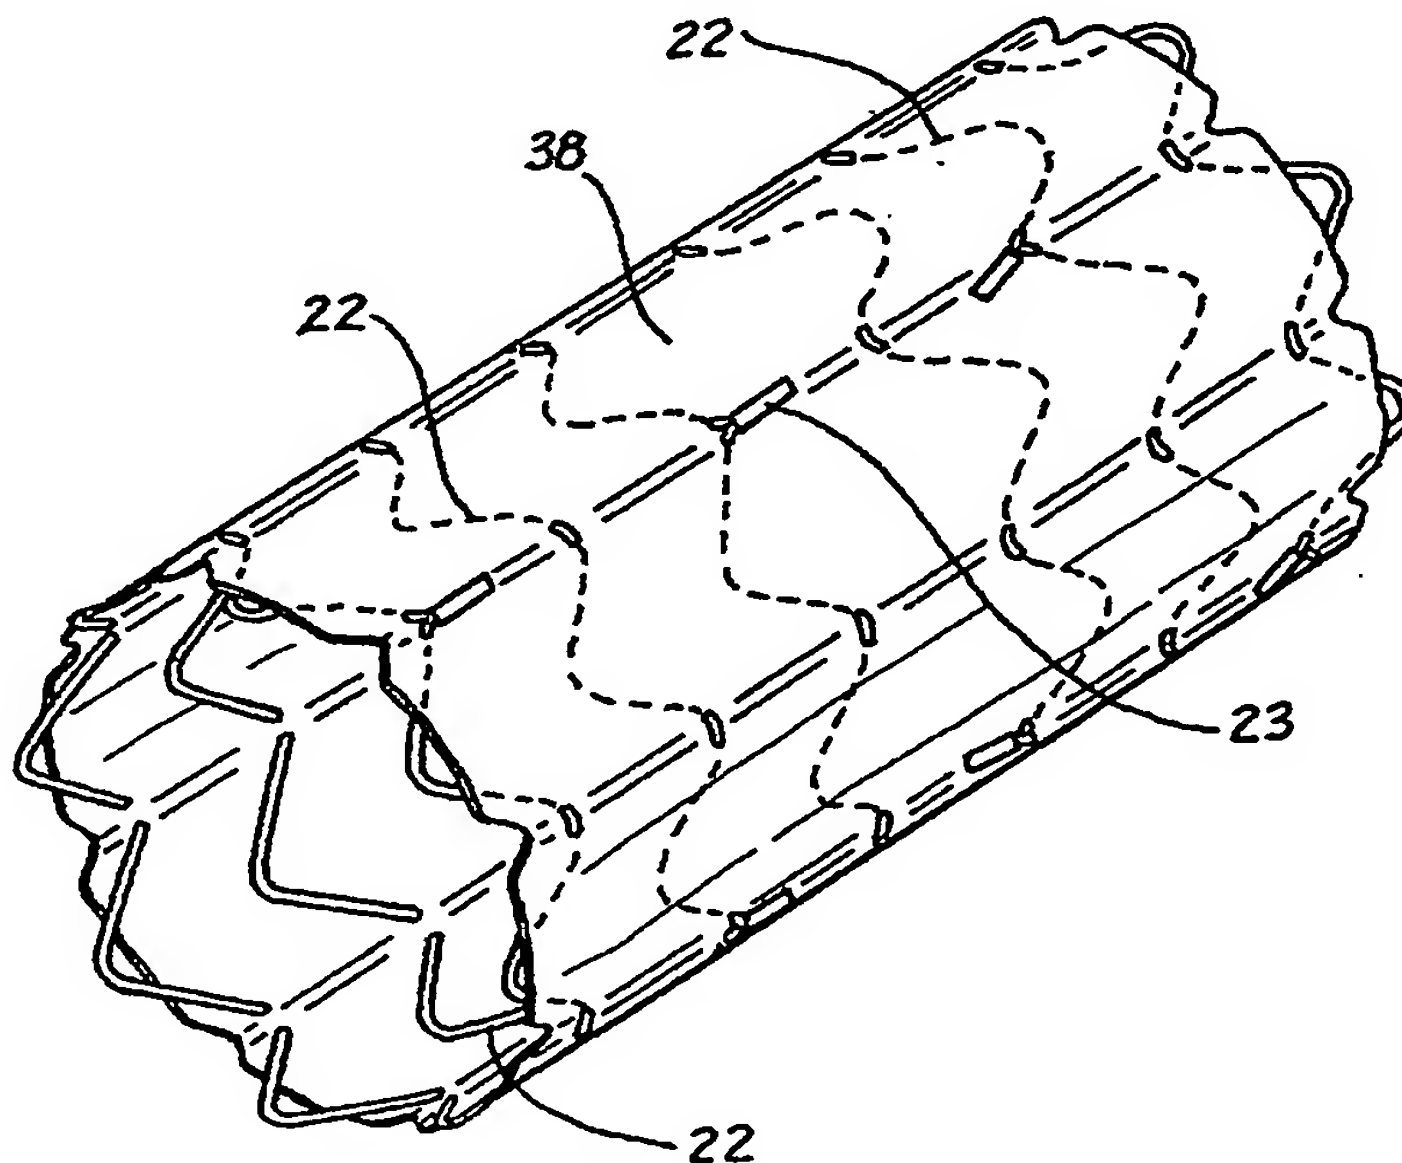

(57) Abstract: Supplemental intraluminal graft extension achieved by cuff-means substantially fortify and enhance endovascularly emplaced systems, particularly for bridging aneurysms. Multiple embodiments based upon overlapping of at least two segments are taught. Cuff-means likewise have applications to restore patency to, or substantially enhance, prior failing emplacements of both home-made and other commercial devices.



*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

**DOUBLE LAYERED INTRALUMINAL GRAFT**

The present invention depends from Australian Provisional Patent Application No. PQ 3027, filed 23 September 1999 in the Commonwealth of Australia, full Paris Convention  
5 priority is hereby earnestly solicited and reserved.

**Field of the Invention**

The present invention relates to an intraluminal device for use in the treatment of  
10 aneurysmal or stenotic disease.

**Background of the Invention**

It is known to use intraluminal grafts and stents of various designs for the treatment of  
15 aneurysms such as aortic aneurysms and occlusive diseases affecting the vasculature or other vessels comprising, inter alia, the hepatobiliary and genito-urinary tracts (which are all hereinafter "vessels"). It is known to form such an intraluminal device of a sleeve in which is disposed a plurality of self-expanding wire stents (see Balko A. et al (1986) Transfemoral Placement of Intraluminal Polyurethane Prosthesis for Abdominal Aortic Aneurysms, 40  
20 Journal of Surgical Research 40, 305-309; Mirich D. et al. (1989) Percutaneously Placed Endovascular Grafts for Aortic Aneurysms: Feasibility Study 170(3) Radiology 170(3), 1033-1037).

In the past, such devices have commonly been used in the treatment of aneurysms, see, for example, US Letters Patents Numbers 5782904, 5968068, 5976192, 6013092, and U.  
25 S. Ser No. 09/203998 all subject to assignment to the entity owning all rights in the instant subject matter. However, it has been recognized that it is within the ambit of some such devices that they also be used to treat stenotic lesions. Whatever the purpose for which an intraluminal device is being used, it has the capacity to be inserted percutaneously through a distal (or proximal) and connecting vessel to that in which the device is to be used. For  
30 example, the device may be inserted through the femoral artery in a catheter, where the device is intended to be used in the treatment of a lesion within the aorta. Upon release of the device from the catheter it may expand to a desirable size, and may extend above and below the lesion thereby bridging that lesion. This method of inserting the device into the body of a patient is applicable where the invention is used in the treatment of aneurysmal disease or  
35 stenotic disease.

Further, where the device is used in the treatment of an aneurysm which extends from a single vessel into one or more divergent vessels, a bifurcated or "trouser graft" is required as described in, for example, Australian Application No 74862/96, and U. S. Ser. No. 09/204699, 09/392655, 09/478352, and 09/478413 each of which is expressly incorporated  
5 herein by reference and subject to assignment to a common entity.

There may be a number of problems associated with such known intraluminal devices which may include rupture of the intraluminal graft due to general wear or damage upon insertion into the vessel. While thicker and more durable grafts may be designed to overcome this problem, such grafts in turn require a larger sized catheter for delivery into the  
10 affected vessel. The limitation in this regard is the size of the artery in which the catheter is being inserted. For example in the situation where a graft is inserted to bridge an aneurysm in the thoracic aorta, the catheter bearing the graft must be inserted through one of the femoral arteries, moved through the femoral artery, into the common iliac artery and eventually into the aorta. If the catheter is too large in diameter, it is not suitable for insertion  
15 into the femoral artery of a patient.

Further, in so-called "trouser grafts", the graft may have a tendency to "kink" in an area of the graft immediately above the area of bifurcation. Whilst kinking in this region may be overcome by adding further reinforcing wires integral the material of the graft in this region, this may increase the diameter of the graft and thus a larger size of catheter may be  
20 required to introduce the graft into the vessel.

The present invention is directed to an alternative form of intraluminal device which in preferred forms may overcome the above problems and in fact has been revised and novel enhanced iterations advanced to the market for the first time post-1999. Likewise further embodiments are yet to be released.

25

### **Summary of the Invention**

In a first aspect, the present invention consists in an intraluminal device comprising a first tubular graft body and at least a second tubular graft body, each tubular graft body  
30 having a length and a first and at least second end wherein when the intraluminal device is disposed within a vessel of a patient, a majority of the length of the second tubular graft body overlaps with a majority of the length of the first tubular graft body.

In yet another aspect, the invention consists in a method for positioning a first and at least a second tubular graft segment, cuff, or body in a vessel of a patient's body, the method including the steps of introducing a catheter into the vessel in the body, causing the first tubular graft member to be moved through the catheter until it extends into the vessel from the proximal end of the catheter, urging the first tubular graft body into contact with the wall of the vessel; causing the second tubular graft member to be moved through the catheter until a substantial length of the second tubular graft body overlaps a substantial length of the first tubular graft body and urging the second tubular graft body into contact with the first tubular graft body.

10 In an embodiment of this further aspect for example, the first tubular graft body is moved through the catheter on an inflatable balloon until it extends into the vessel from the proximal end of the catheter. The balloon is then inflated to cause the first tubular graft body to be urged into contact with the wall of the vessel and subsequently deflated and withdrawn from the vessel. The second tubular graft body is then moved through the catheter on an inflatable balloon until a substantial length of the second tubular graft body overlaps a substantial length of the second tubular graft body and the balloon inflated such that the second tubular graft body is urged into contact with the first tubular graft body. The balloon is then deflated and the catheter withdrawn from the vessel. Alternatively, the first tubular graft body is moved through the catheter until it extends into the vessel. A balloon may then be passed through the catheter until it extends from the proximal end of the catheter internal the first tubular graft body whereupon the balloon is inflated to cause the first tubular graft body to be urged into contact with the wall of the vessel. The second tubular graft body may be similarly introduced into the vessel.

25 In yet another embodiment, in place of a balloon, the first and the second tubular graft bodies may be self expandable such that when the tubular graft body extends from the proximal end of the catheter it takes on an expanded configuration such that it is caused to contact the vessel wall.

30 In examples based on at least one embodiment, the first and the second tubular graft bodies have an equal cross sectional area or a different cross sectional area before insertion into the vessel of a patient. When *in situ*, however, typically the maximum cross sectional area of the first tubular graft is greater than the maximum cross sectional area of the second tubular graft body. Accordingly, the first tubular graft body is inserted into the vessel of a

patient and the second tubular graft body inserted internal the first tubular graft body such that a substantial portion of the second tubular graft body overlaps with a substantial portion of the first tubular graft body. Alternatively, the maximum cross sectional area of the first tubular graft body may be less than the maximum cross sectional area of the second tubular graft body such that upon placement of the first tubular graft body within the vessel of a patient, the second tubular graft body is introduced such that the second tubular graft body is placed external to the first tubular graft body.

In one illustrated embodiment, the entire length of the second tubular graft body is overlapped with a length of the first tubular graft body.

In a further illustrated embodiment the entire length of the first tubular graft body is overlapped with a length of the second tubular graft body.

In yet a further illustrated embodiment, the first and second tubular graft bodies are of the same length and the entire length of the second tubular graft body is overlapped with the entire length of the first tubular graft body.

Prototypes of related iterations have been used and tested. According to yet a still further embodiment, the area of overlap of the two tubular graft bodies is greater than 50% of the length of the tubular graft bodies. More preferably, the area of overlap is greater than 75-80% and more preferably still between 80 and 100%.

In a still further embodiment, a portion of the second tubular graft body does not overlap with the first tubular graft body, said non-overlapping portion extending longitudinally from the first tubular graft member into the lumen of the vessel in which the device is disposed.

In one tested and working embodiment, the first and at least second tubular graft bodies are circumferentially reinforced along their length by a plurality of separate, spaced apart, malleable wires. Each of the wires can have a generally closed sinusoidal shape.

In still a further embodiment, the first and second tubular graft bodies are longitudinally reinforced along their length by a longitudinally reinforcing malleable wire. The longitudinally reinforcing wire may be positioned between two circumferentially reinforcing wires. Several longitudinally reinforcing wires may be positioned along the length of both the first and the second tubular graft bodies. Each wire may be generally straight in shape or may have a zig-zag or sinusoidal shape. The presence of a longitudinally reinforcing wire has the advantage of reinforcing the tubular graft bodies such that neither



tubular graft body is forced into a compressed state along its longitudinal axis.

In a still further embodiment, one of the tubular graft bodies (for example, the first) may be longitudinally reinforced, said tubular graft body having no circumferential reinforcement. In this embodiment the other (for example, the second) tubular graft body is circumferentially reinforced, said other tubular graft body having no longitudinal reinforcement.

In another alternate embodiment, the first and at least second tubular graft bodies are circumferentially reinforced along their length by one continuous wire, the wire taking on a spiral configuration along the length of both the first and at least second tubular graft bodies. Likewise, helices in the configuration of the wire are within the scope of the instant techniques.

In another embodiment, the first and at least second tubular graft bodies are circumferentially reinforced along their length by a series of wires or one continuous wires woven into the material of the tubular graft bodies such that the wires are not exposed at either the outer or the inner surface of the tubular graft bodies. Such an enclosed wireform arrangement is particularly useful in one embodiment of the invention wherein the tubular graft body is inserted into the vessel of a patient and caused to expand within the vessel of the patient by way of an inflatable balloon. In a further embodiment wherein the tubular graft body is adapted to self expand without the need for a balloon it is not required that the wires be entirely enclosed and indeed it is preferred that at least a portion of the wires are positioned on either the outside or the inside surfaces of the tubular graft bodies. Like wise, it is known to artisans that, for example, any techniques in the commonly owned or assigned patents and patent applications such as interweaving of wireforms having predetermined or pre-ordained spatial orientations made of, for example, Elgiloy<sup>®</sup> wireforms with Dacron<sup>®</sup> grafts (available from Baxter Vascular Systems Division, Irvine, California) or a PTFE (Baxter Healthcare Corporation, Laguna Hills, California) and Nitinol<sup>™</sup> (Memry Metal, California) are equally applicable and work well within human patients.

In a further embodiment, both tubular graft bodies are either balloon expandable or self expandable. Alternatively, one of the tubular graft bodies may be balloon expandable and the other tubular graft body self expandable. Preferably, when in situ within the vessel of a patient the outer tubular graft body (for example, the first tubular graft body) which is in contact with the vessel wall is of the self expandable type and the inner tubular graft body

(for example the second tubular graft body) is of the balloon expandable type.

In a still further embodiment, at least a portion of the length of one tubular graft body may be adapted to be balloon expandable and the remaining length of the same tubular graft body adapted to be self expandable. In a particularly preferred embodiment, the first end of the tubular graft body is self expandable and the remainder of the tubular graft body is balloon expandable. This embodiment is of particular significance when it is understood that misplacing of a balloon internal the tubular graft body such that the balloon extends past the first end of the tubular graft body may cause inflation of the vessel wall itself and may potentially result in rupture of the vessel wall. With the first end of the tubular graft body adapted such that it is self expandable, the balloon need not be inserted as far towards the first end thereby reducing the risk of over extension of the balloon and subsequent damage of the vessel wall.

In a further embodiment, the first and at least second tubular graft bodies are reinforced along their length by a series of separate spaced apart stents. Alternatively in another embodiment, at least some of the stents may be interconnected or all of the stents may be interconnected to form one continuous stent.

In still a further embodiment, the first tubular graft body includes at least one first engagement member which is connected to or integral with a wall of the first tubular graft body at a position intermediate the ends of the first tubular graft body.

In yet a further embodiment, the at least one first engagement member is adapted to extend externally of the wall of the first tubular graft body. When disposed in a vessel, the engagement member preferably abuts the surrounding vessel wall thereby securing the first tubular graft body within the vessel.

In another embodiment, the at least one first engagement member comprises the ends of the malleable wires which are joined together to form a tail means. Each tail means is preferably on the outside of the graft body and positioned to lie along its radially outer surface. The ends may be joined by welding, by being twisted together or in any other suitable manner. The ends of adjacent wires preferably project in generally opposite directions along the first tubular graft body and when the first tubular graft body is inserted into a vessel those wires that engage the vessel wall will assist in preventing dislodgement of the first tubular graft body within the vessel.



In a further embodiment, several of the tails of the malleable wires may be on or adjacent an inside wall of the first tubular graft body such that upon insertion of the second tubular graft body internal the first tubular graft body, the tails engage with the wall of the second tubular graft body thereby securing the second tubular graft body in place. Frictional, mechanical, and frustoconical means for engaging are further used with the overlapping aspects of the present invention.

In another embodiment, the at least one first engagement member comprises a hook-like member adapted to project from at least the first end of the first tubular graft body, when disposed in a vessel, the hook-like member preferably engages the wall of the vessel in which the first tubular graft body is disposed thereby preventing dislodgement of the first tubular graft body within the vessel. Alternatively, the first tubular graft body includes a stent or a series of spaced apart stents which form a framework to which may be attached an endoluminal graft. Expansion of the stent or stents will cause the first tubular graft body to expand and press against the wall of a vessel into which it has been placed thereby securing the first tubular graft body in that vessel.

In yet a further embodiment, the first tubular graft body includes at least one second engagement member positioned intermediate the two ends of the first tubular graft body, the at least one second engagement member is adapted to project into the lumen of the first tubular graft body such that it engages the wall of the second tubular graft body.

In one embodiment, the at least one second engagement member preferably includes a ring-like member adapted to project into the lumen of the first tubular graft body from the inner surface of the first tubular graft body.

In a further embodiment, the ring-like member is continuous or discontinuous in configuration.

Alternatively, in a further embodiment, the second engagement member could include hook-like members circumferentially disposed around the inner surface of the first tubular graft body. In another form, the tails formed from the ends of the separate, spaced apart malleable wires could be adapted to project into the lumen of the first tubular graft body such that they engage with the second tubular graft body, thereby securing the second tubular graft body within the lumen of the first tubular graft body.

In one embodiment, the first tubular body comprises a simple tubular sheath adapted to be disposed in a vessel such that it engages with and is attached to the wall of the vessel.

In a further embodiment, the at least second tubular graft is preferably formed of a more durable and thick material than that of the first tubular graft body, for example Dacron<sup>®</sup> or polytetrafluoroethylene (PTFE).

5 In yet a further embodiment, the surfaces of both the first and the second tubular graft bodies are coated with a material from the group comprising biocompatible glues, adhesives, or the like engineered cellular matrices for joining surfaces.. The biocompatible glue or the like adhesion means enhances attachment of the first tubular graft body to a vessel wall thereby further preventing dislodgement of the intraluminal device within the vessel and further enhancing attachment of the second tubular graft body to the first tubular graft body.

10 In another embodiment, the surfaces of both the first and second tubular graft bodies may be coated with fibrins or some other material to stimulate fibrin or cellular ingrowth into the device from the surrounding tissue. Such ingrowth further secures the intraluminal device within the vessel wall. An example of a material which increases tissue ingrowth into the tubular graft bodies is polyurethane. Alternatively, a polyurethane/polycarbonate composite  
15 may be used to enhance cellular ingrowth.

In a further embodiment, the first and at least one second tubular graft bodies include a collar member attached to the first end. In addition, a further collar member may be attached to the at least one second end of the tubular graft bodies.

In another embodiment, the collar member is not attached to the tubular graft bodies  
20 but is inserted separately from the tubular graft bodies.

The surface of the collar member may be coated with fibrins or some other material such as polyurethane or polyurethane/polycarbonate composite and adapted to stimulate cellular ingrowth into the device from the surrounding tissue.

In a further embodiment, the first tubular graft body is circumferentially reinforced by  
25 a series of separate, spaced apart malleable wires along only a portion of its length.

In alternately, yet still another embodiment, the second tubular graft body is circumferentially reinforced by a series of separate, spaced apart malleable wires along only a portion of its length, see for example United States Serial No. 09/163,831 which has been expressly incorporated by reference herein.

30 In a further embodiment, when the device of the invention is *in situ* within the vessel of a patient, the portion of the first tubular graft body that is not reinforced overlaps with the portion of the second tubular graft body that is reinforced and the portion of the second

tubular graft body that is not reinforced overlaps with the portion of the first tubular graft body that is reinforced. In this case, the entire length of the device will be reinforced.

In yet a further embodiment, when the device is *in situ* within a vessel of a patient, only a superior portion of the first tubular graft body distal its own entry point is  
5 circumferentially reinforced by the wires and only an inferior portion of the second tubular graft body proximal its entry point is reinforced by the wires such that the overlapping of first and second tubular graft bodies causes the entire length of the device to be circumferentially reinforced. The circumferential reinforcement of each tubular graft body is not, however, limited to circumferential reinforcement of the superior or inferior portions of each tubular  
10 graft body and is simply adapted such that *in situ*, a length of the device that is not reinforced by the separate spaced apart malleable wires located on the first tubular graft body is reinforced by separate, spaced apart, malleable wires located on the second tubular graft body.

The intraluminal device according to this invention may be used to treat aneurysmal  
15 or occlusive disease. In addition to treating aortic aneurysms they are particularly suitable for treating aneurysms of the femoral artery, the popliteal artery, the thoracic segment of the aorta, the visceral arteries such as the renal and mesenteric arteries, the iliac and subclavian artery.

It is sometimes the case that the aneurysm extends to or slightly beyond an arterial  
20 bifurcation. In such a case, the second tubular graft body is adapted such that it is bifurcated at its downstream end, a so-called "trouser graft". A supplemental graft, or cuff-means may then be introduced through each of the subsidiary arteries and overlapped with the respective lumenae of the bifurcated part of the second tubular graft body. For instance, in the case of an aneurysm in the aorta that extends into one or each of the iliac arteries, the second tubular  
25 graft body would be placed in the aorta through one of the iliac arteries. Supplemental grafts which dock with the bifurcated end of the primary graft would then be inserted through each of the iliac arteries. In such a case the region of graft body directly superior the bifurcated region of the second tubular graft body can have a propensity to occasionally kink. The overlapping of the first and second tubular graft bodies, therefore, increases the  
30 circumferential reinforcement in the region of the device superior the bifurcated region by increasing the number of separate, spaced apart, malleable wires or other reinforcing wires thereby reducing the likelihood of kinking in this region. In a further embodiment, the first

and at least second tubular graft bodies are longitudinally reinforced in addition to or instead of being circumferentially reinforced.

In a further embodiment of the first and second aspects of the invention, the second tubular graft body is inserted into the lumen of the first tubular graft body such that a  
5 substantial length of the second tubular graft body overlaps with a substantial length of the first tubular graft body.

In still a further embodiment of the second aspect of the invention, the second tubular graft body is of the "trouser graft" type such that the bifurcated portion is positioned such that it extends longitudinally from the first tubular graft body into the surrounding vessel, for  
10 example, the aorta and wherein a supplemental graft may be introduced through each of the subsidiary arteries and overlapped with the respective lumenae of the bifurcated portion of the second tubular graft body.

In another embodiment, where the intraluminal device is adapted to span an aneurysm affecting an area of artery which is bifurcated, both the tubular graft bodies are of the "trouser  
15 graft" variety. Accordingly, the tubular graft bodies comprise a main body positioned in, for example, the aorta and two leg members adapted to extend into the iliac arteries. The first leg member of the first tubular graft body may be shorter than the second leg member. In this case, the second leg member of the second tubular graft member is shorter than the first leg member of the second tubular graft member. Accordingly, the two tubular graft members  
20 may be mirror images of each other or as close to mirror images as is practicable. This has the advantage of avoiding unnecessary bulking in the leg members of the graft due to excessive overlapping of the two grafts in this area. Because the main bodies of each tubular graft body overlap with each other, however, the intraluminal device is still reinforced in the area of the device most likely to kink, that is, the area directly above the bifurcation of the  
25 tubular graft bodies.

In a further embodiment, the first tubular graft body may include only one leg member, the first tubular graft body having an aperture rather than a second leg member. In this case, the second tubular member is adapted such that it has one leg member that may be inserted through the aperture of the first tubular graft body. In place of the second leg  
30 member, the second tubular member has an aperture through which the leg member of the first tubular graft body may be inserted. This embodiment has the advantage that each tubular graft member is symmetrical in shape. Typically, with trouser grafts, the tubular graft

body must be positioned in a certain orientation, such that one leg member extends into one vessel and the other leg member extends into another vessel. In the case of a graft for bridging an aneurysm spanning the bifurcation of the aorta into the iliac arteries, one of the leg members will extend towards or into the left iliac artery and the other leg member will extend towards or into the right iliac artery. Radio-opaque markers positioned on the graft are typically used to ensure the correct positioning of the graft. In the present embodiment, however, because the first tubular graft body is symmetrical in shape there is no need to use such markers to ensure correct positioning of the tubular graft body and the one leg member will extend towards or into the desired iliac artery. A second tubular graft member may then be inserted, the second tubular graft member having one leg member that extends towards or into the other iliac artery.

According to a feature of the present invention, there is provided in an endovascularly emplaced prosthesis for bridging an aneurysm, the improvement which comprises; at least a supplemental graft member positioned whereby a flow path through a treated vessel is extended.

According to another feature of the present invention, there is provided, an apparatus for intraluminal emplacement comprising; a first tubular body; and a second tubular body wherein each said tubular body further comprises a graft having a length and a first and at least a second end, whereby when the apparatus is disposed within a vessel of a patient, a predetermined length of the second graft body overlaps with a desired length of the first graft body.

According to yet still another feature of the present invention, there is provided a method of intraluminal emplacement comprising:

providing a first graft body and positioning a cuff-means for extending the first graft body within said first graft body for affixing said cuff-means whereby a lumen of said first graft body is extended.

#### **Brief Description of the Drawings**

Hereinafter by way of example is a preferred embodiment of the present invention described with reference to the accompanying drawings, in which:

Figure 1 is a diagrammatic partially cut-away ventral view of a patient with an aortic

aneurysm which has been bridged by an intraluminal graft according to an embodiment of the present invention.

Figure 2 is a detailed longitudinal sectional view of the intraluminal device of Figure 1.

5 Figure 3 is a detailed elevational view of one end of an intraluminal device of an embodiment of the invention.

Figure 4 is a detailed view of one component of one embodiment of the invention.

Figure 5 is a detailed view of one component of a further embodiment of the invention.

10 Figure 6 is a side elevational view of a device of the present invention showing the spatial arrangement between the components of the device, according to an embodiment of the present invention.

Figure 7 is a detailed view of one component of a further embodiment of the invention.

15 Figure 8 is a side elevational view of one embodiment of the invention.

Figure 9 is a side elevational view of one component of the embodiment of the invention depicted in Figure 8.

Figure 10 is a side elevational view of another component of the embodiment of the invention depicted in Figure 8.

20 Figure 11 is a more detailed side elevational view of the embodiment of the invention as depicted in Figure 8.

Figure 12 is a schematic view of a further embodiment of the invention.

Figure 13 is a side elevational view of another embodiment of the invention.

25 Figure 14 shows a supplemental cuff-means according to an embodiment of the present invention.

### **Description of the Preferred Embodiments**

30 An intraluminal device according to the present invention is generally shown as 10 in the drawings. The intraluminal device 10 comprises two separate components, a first graft 11 and a second graft 12.

The device 10 is adapted for insertion transfemorally into a patient to achieve



bridging and occlusion of an aneurysm 13 present in the aorta 14. As shown in Fig 1, the aorta 14 bifurcates to form the common iliac arteries 15 which in turn divide into the internal 16 and external 17 iliac arteries. The external iliac artery in turn forms the femoral artery 18. The first graft 11 is inserted inside a catheter (not shown) and introduced into one of the  
5 femoral arteries 18 in a leg of a patient. Once the catheter is located appropriately with its proximal end in the aorta 14, the first graft 11 is ejected from the catheter and expanded using a balloon so that the first graft 11 is in intimate contact along its length and around its full periphery with the surrounding vessel. The first graft 11 then bridges the aneurysm. Alternatively, in a preferred embodiment, the first graft 11 is made from a self expandable  
10 material such that first graft 11 is in a collapsed configuration internal the catheter. Upon ejection from the catheter, the first graft takes on an expanded configuration such that the first graft 11 is in intimate contact along its length and around its full periphery with the surrounding vessel.

In one embodiment, the first graft 11 comprises a tube made from a very thin material  
15 and is used essentially as an anchor for the second more durable graft 12. To assist in the placement of the first graft 11 in the aorta 14, the first graft 11 is provided with engagement members 19 (see Fig. 5) which project from one end 21 of the first graft 11. It is to be recognised that further engagement members may be circumferentially disposed along the entire length of the first graft 11.

20 The first graft 11 and second graft 12 may be circumferentially reinforced along their lengths by a number of separate and spaced wires 22. The wires are preferably as thin as possible and are malleable such that they may be bent to any desired shape. The wires are each woven into the fabric of the first graft 11 or second graft 12 such that alternate crests of each wire 22 are outside of the graft with the remainder of the wire 22 inside the graft. The  
25 ends of each wire 22 are located outside the first graft 11 or second graft 12 and are twisted together to form a tail 23. The tails or alternate wires may be bent in opposite longitudinal directions along the outside of the surface of the first graft 11. The arrangement of the tails 23 on the outside of the first graft 11 assists in the positioning of the first graft 11 in the aorta as the tails 23 have a tendency to abut against the wall of the aorta thereby securing the first  
30 graft 11 within the aorta.

In a further embodiment, the first graft 11 and the second graft 12 may be longitudinally reinforced by wire 36. Figure 13 depicts the longitudinal reinforcement of the

first graft 11 only but it is readily envisaged that second graft 12 may be similarly reinforced. Further, wire 36 is shown as being connected to the circumferentially reinforcing wires 22. It is to be understood that wire 36 may be connected to the material of the first graft 11 and not to the wires 22. Wire 36 may be straight or zig-zag in shape or may be a sinusoidal shape as depicted in Figure 13.

Once the first graft 11 is in position, the second graft 12 is similarly introduced into the aorta 14 by way of insertion of a catheter through the femoral artery 18 of a patient. In the depicted embodiment, the second graft 12 is of the "trouser graft" type, that is, it has a main body 24 and a bifurcated portion 25 and is made from woven Dacron®. The catheter is introduced into the lumen of the first graft 11 and the second graft 12 inflated by way of a balloon such that the main body 24 expands and abuts against the inner facing surface of the first graft 11. The bifurcated portion 25 extends in a longitudinal plane from the other end 26 of the first graft 11 into the lumen of the aorta 14.

The first graft 11 may be provided with internal rings 27 which act to overlay the wires 22 of the second graft 12 and thereby secure the second graft 12 in place within the lumen of the first graft 11.

Figure 8 to 10 depict a further embodiment of the invention wherein both graft 11 and 12 are "trouser grafts". The first graft 11 has a main body 24, a long leg 28 and a short leg 29. The second graft 12 also has a main body 24, a long leg 31 and a short leg 32. When the two grafts are in situ within a vessel of a patient, as depicted in Figure 11, the main body 24 of each graft overlap with each other entirely whereas overlapping of the legs of the grafts is kept to a minimum to avoid unnecessary "bulking" of the graft in this area.

In another embodiment depicted in Figure 12, the first graft 11 has a main body 24 and one leg 33. A second leg is absent in this embodiment, and in its place is simply an aperture 34. A second graft 12 may be inserted internal the first graft 11 such a leg 35 of the second graft 12 extends through aperture 34. The leg 35 of second graft 12 extending through aperture 34 is shown in phantom in Figure 12.

Referring now to Fig. 14, supplemental cuff-means 38 likewise comprises a plurality of crimped stent-formed wires 22 which are each woven into the fabric of supplemental graft 38 such that alternate crests of each wire 22 are outside of graft 38 with the remainder of the wire 22 inside the graft. The ends of each wire 22 are located outside graft 38 and are twisted together to form a tail 23. The tails or alternate wires may be bent in opposite longitudinal

directions along the outside of the surface of graft 38. The arrangement of the tails 23 on the outside of graft 38 assists in the positioning of graft 38 in the aorta as the tails 23 have a tendency to abut against the wall of the aorta thereby securing graft 38 within the aorta.

Likewise, those having a modicum of skill in the art will understand that supplemental  
5 cuff-means or graft 38 is effective for use within the (failed or leaking) grafts of other commercial entities, such as, for example, the GUIDANT/EVT brand ANCURE® DEVICE; the GORE brand EXCLUDER®; the Boston Scientific Vanguard® brand; Medtronic/AVE ANERUERX® or TALENT® brand devices in addition to those of the Cook Endovascular Graft brand ZENITH™ AAA Endovascular Graft. It is noted that specific overlapping,  
10 sizing, and the like dimensional parameters will be obvious to artisans.

It will be appreciated by persons skilled in the art that numerous variations and/or modifications may be made to the invention as shown in the specific embodiments without departing from the spirit or scope of the invention as broadly described. The present  
15 embodiments are, therefore, to be considered in all respects as illustrative and not restrictive.

20

25

30

**WHAT IS CLAIMED IS:**

- 1           1.       In an endovascularly emplaced prosthesis for bridging an aneurysm, the  
2                   improvement which comprises:  
3                   at least a supplemental graft member positioned whereby a flow path  
4                   through a treated vessel is extended.
  
- 1           2.       An apparatus for intraluminal emplacement comprising:  
2                   a first tubular body; and  
3                   a second tubular body;  
4                   wherein each said tubular body further comprises a graft having a length  
5                   and a first and at least a second end, whereby when the apparatus is disposed  
6                   within a vessel of a patient, a predetermined length of the second graft body  
7                   overlaps with a desired length of the first graft body.
  
- 1           3.       A method of intraluminal emplacement comprising:  
2                   providing a first graft body;  
3                   positioning a cuff-means for extending the first graft body within said first  
4                   graft body; and  
5                   affixing said cuff-means whereby a lumen of said first graft body is  
6                   extended.
  
- 1           4.       A method for positioning a plurality of intraluminal graft members  
2                   comprising the steps of:  
3                   providing at least two intraluminal graft members comprising a tubular  
4                   graft body having a length, a first end and second end, wherein said graft is  
5                   circumferentially reinforced along its length by a plurality of spaced-apart wires;  
6                   providing a catheter having a proximal end;  
7                   providing an inflatable balloon;  
8                   introducing said catheter into a vessel in the body;

WO 01/21102

PCT/US00/16457

9 causing said intraluminal graft and said inflatable balloon to be carried  
10 with said catheter until said graft and said inflatable balloon extend in the vessel  
11 from said catheter proximal end;  
12 inflating said balloon to cause said wires to be urged into contact with the  
13 wall of the vessel;  
14 deflating said balloon and withdrawing said balloon and said catheter from  
15 the vessel, and, repeating each of said steps for each of the additional  
16 emplacement of a desired number of said at least intraluminal graft members.

1 5. The method of Claim 4, further comprising the step of placing said  
2 intraluminal  
3 graft on said inflatable balloon.

1 6. The method of Claim 4, further comprising the step of inflating said  
2 balloon to expand said graft.

1 7. The method of Claim 4, further comprising the step of radially  
2 compressing said intraluminal graft about said inflatable balloon.

1 8. The method of Claim 4, wherein said intraluminal graft is utilized to  
2 bridge an aneurysm and said method further comprises the step of positioning said  
3 catheter in the vessel so that the proximal end of said catheter is beyond the  
4 proximal end of the aneurysm.

1 9. The method of Claim 4, further comprising selecting the diameter of said  
2 intraluminal graft to be substantially equal to the diameter of the vessel when it is  
3 undistended.

1 10. The method of Claim 4, further comprising selecting the diameter of said  
2 intraluminal graft to be slightly larger than the diameter of the vessel when it is  
3 undistended.

1 11. The method of Claim 4, further comprising the step of inflating said  
2 balloon to cause said wires to be displaced radially outward to restrain said graft  
3 against longitudinal movement relative to the vessel.

1 12. The method of Claim 4, wherein each said graft is circumferentially  
2 reinforced along its length by a plurality of separate, spaced-apart wires.

1 13. A method for positioning an intraluminal graft to treat a region  
2 of a vessel, comprising:  
3 providing an intraluminal graft, into a situs wherein an emplaced graft or  
4 stent exists, comprising a tubular graft body having a length, a first end and  
5 second end, wherein said graft is circumferentially reinforced along its length by a  
6 plurality of spaced-apart wires;  
7 providing an inflatable balloon;  
8 radially compressing said graft on said balloon;  
9 providing a sheath catheter having a proximal end;  
10 inserting said graft and balloon into the end of said sheath catheter;  
11 introducing said catheter into a vessel bridged, at least partially by the  
12 emplaced graft or stent in the body;  
13 causing said intraluminal graft to be carried with said catheter until said  
14 graft extends in the vessel from said catheter proximal end;  
15 withdrawing said sheath catheter to expose said graft and span the region  
16 of the vessel to be treated.

1 14. An intraluminal graft comprising:  
2 a tubular graft body circumferentially reinforced along its length by a  
3 plurality of wires, wherein said graft body comprises at least two layers of a  
4 biocompatible material and wherein said wires are sandwiched between said  
5 layers.

1 15. The intraluminal graft of Claim 5 wherein said tubular graft body is  
2 circumferentially reinforced along its length by a plurality of separate wires.



- 1        16.    The intraluminal graft of Claim 5 wherein said biocompatible material is  
2        Dacron.
- 1        17.    The intraluminal graft of Claim 5 wherein said biocompatible material is  
2        expanded PTFE.
- 1        18.    An intraluminal graft comprising:  
2                a tubular graft body having a length, a first end and second end;  
3                wherein said tubular graft body is circumferentially reinforced along its length  
4                by a plurality of wires which are woven throughout the fabric of the graft.
- 1        19.    A method of manufacturing the intraluminal graft of Claim 5, comprising  
2        the step of:  
3                interweaving said wires with said tubular graft body during its production.
- 1        20.    An intraluminal graft comprising a tubular graft body having a length, a  
2        first end and second end, wherein said tubular graft body is circumferentially  
3        reinforced along its length by a plurality of wires; and  
4                wherein at least said first end of said graft body is provided with a wire  
5        which has alternate apices extending beyond at least said first end of said graft  
6        body to extend across the lumen of a second vessel opening into the first vessel in  
7        which the graft is being placed without occluding that lumen.

1/8

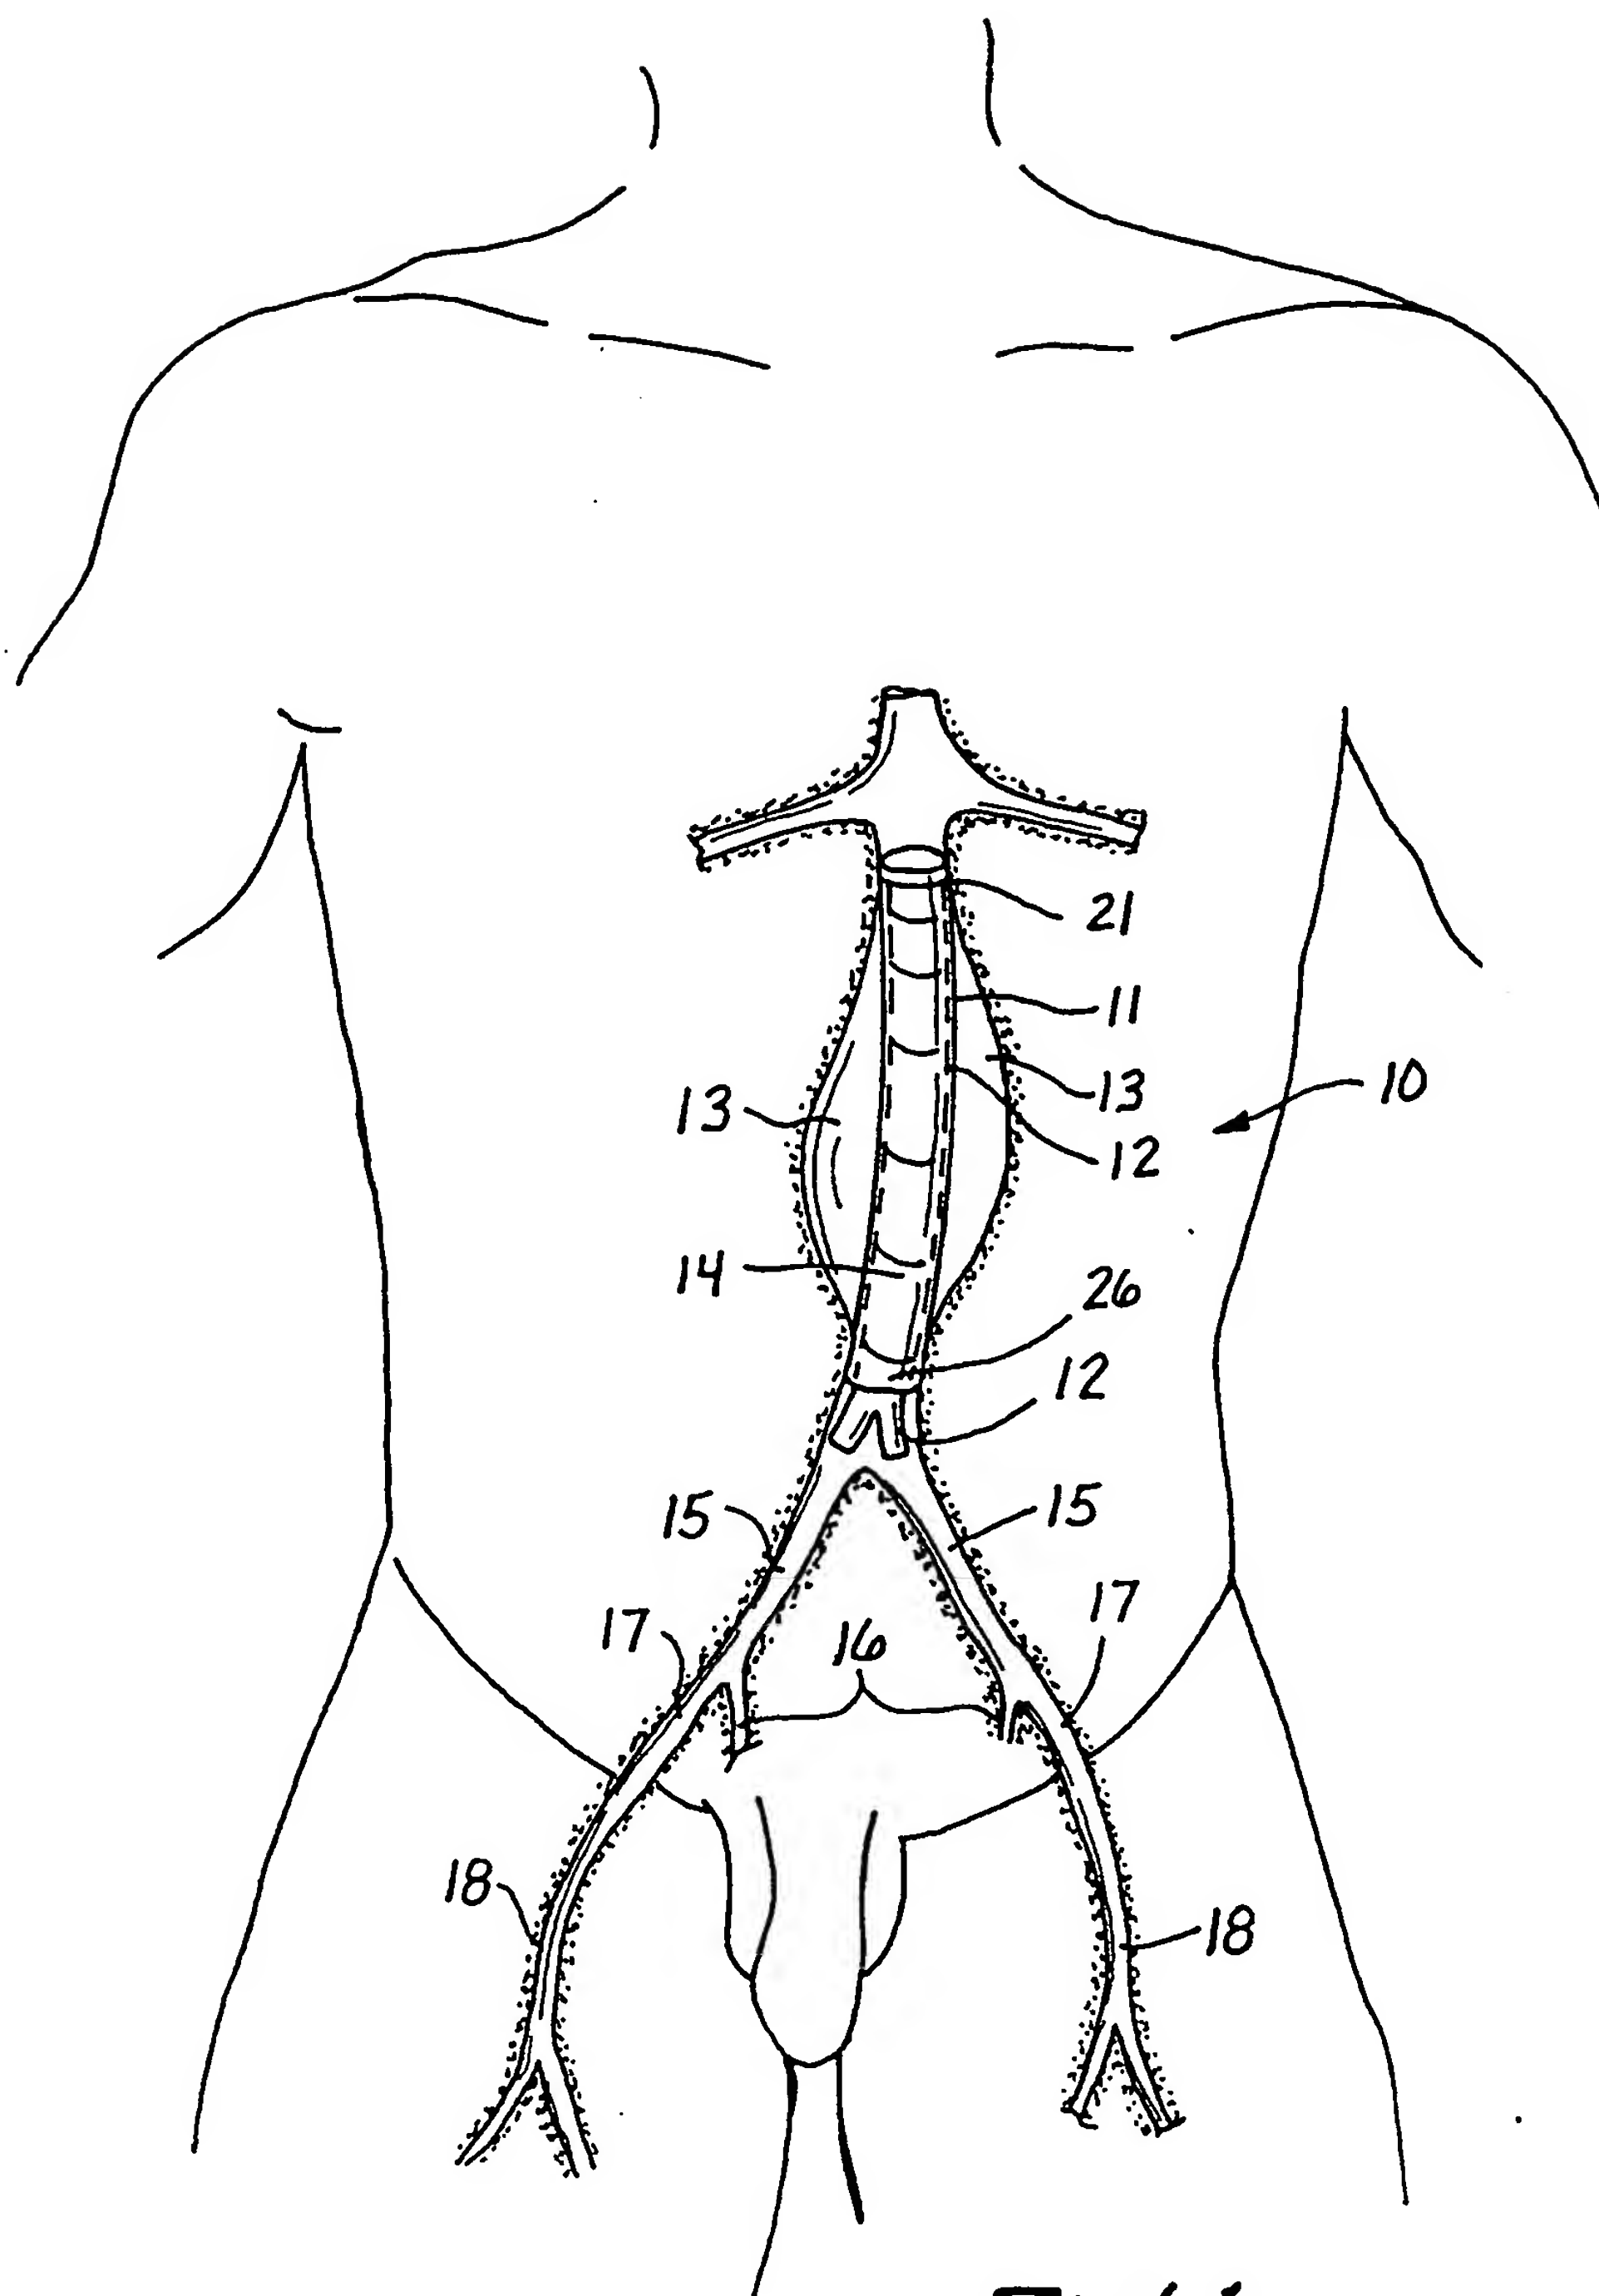


Fig. 1

2/8

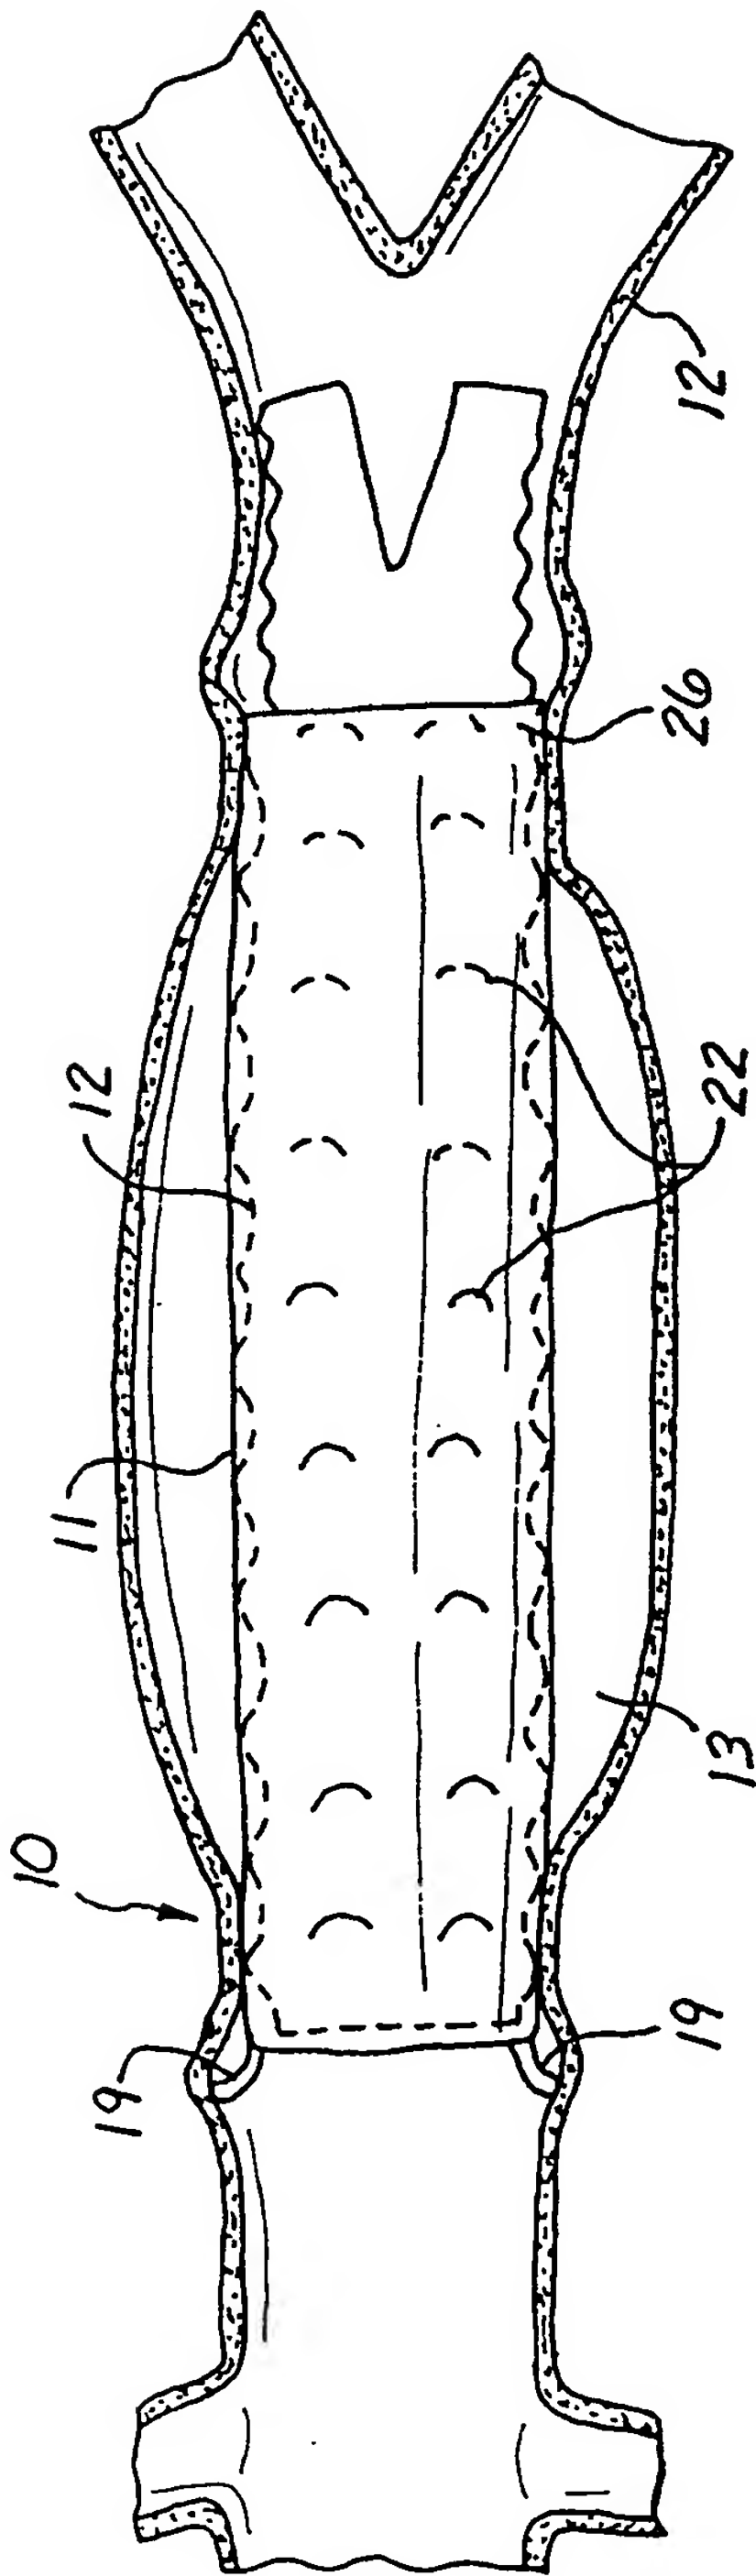


Fig. 2




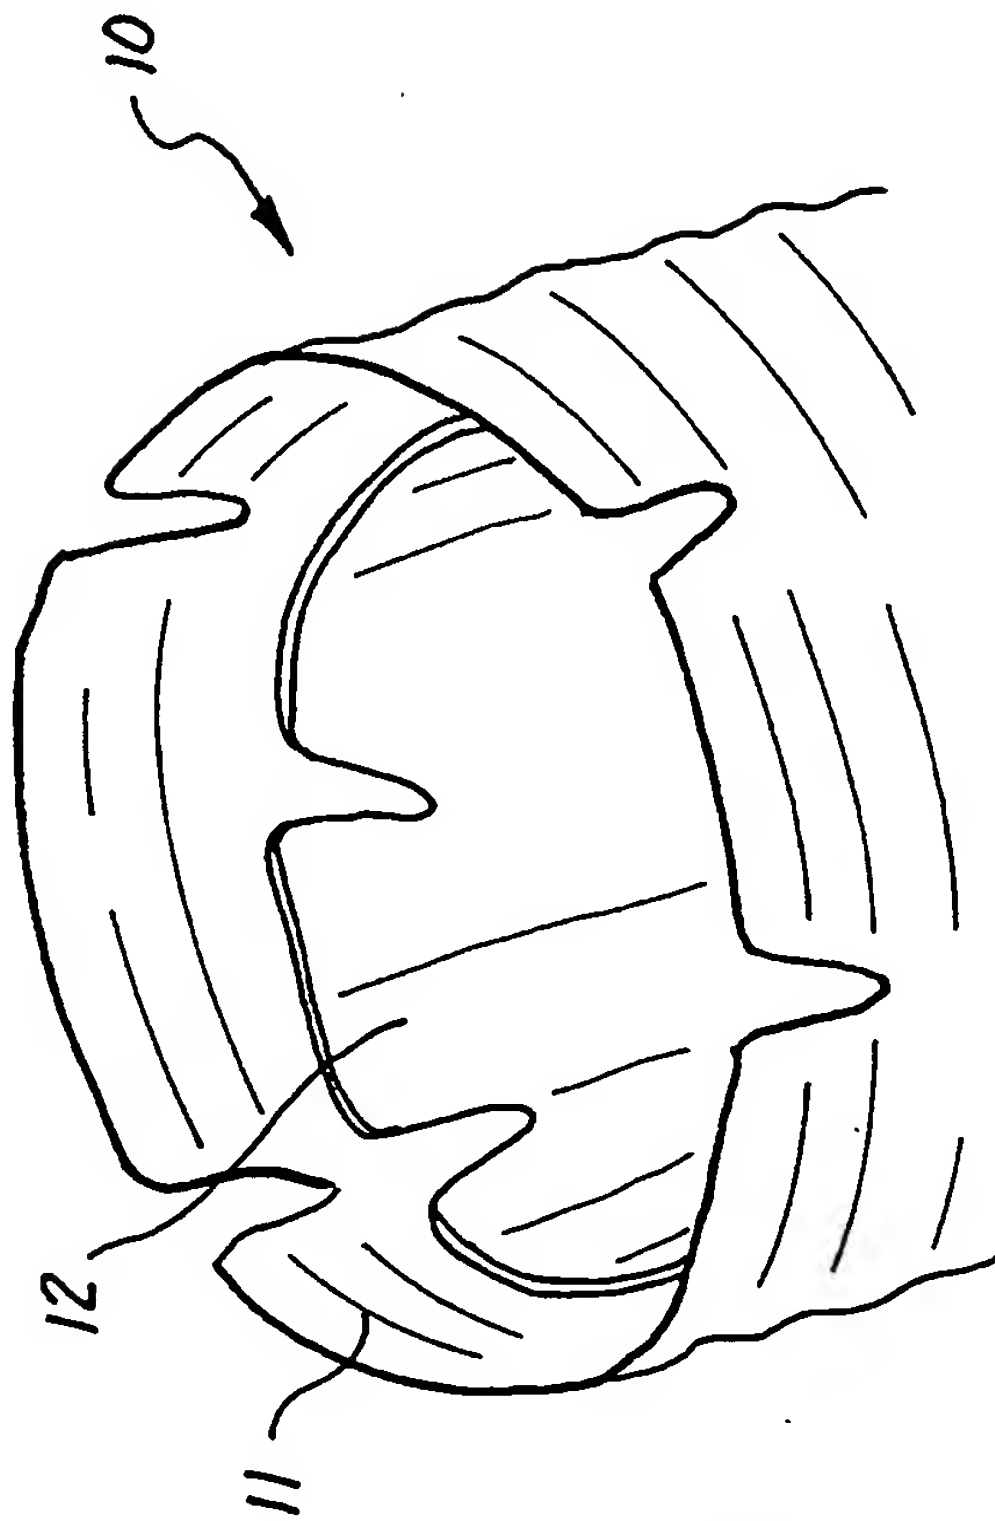


Fig. 3


3/8

*Fig. 4**Fig. 5*

4/8

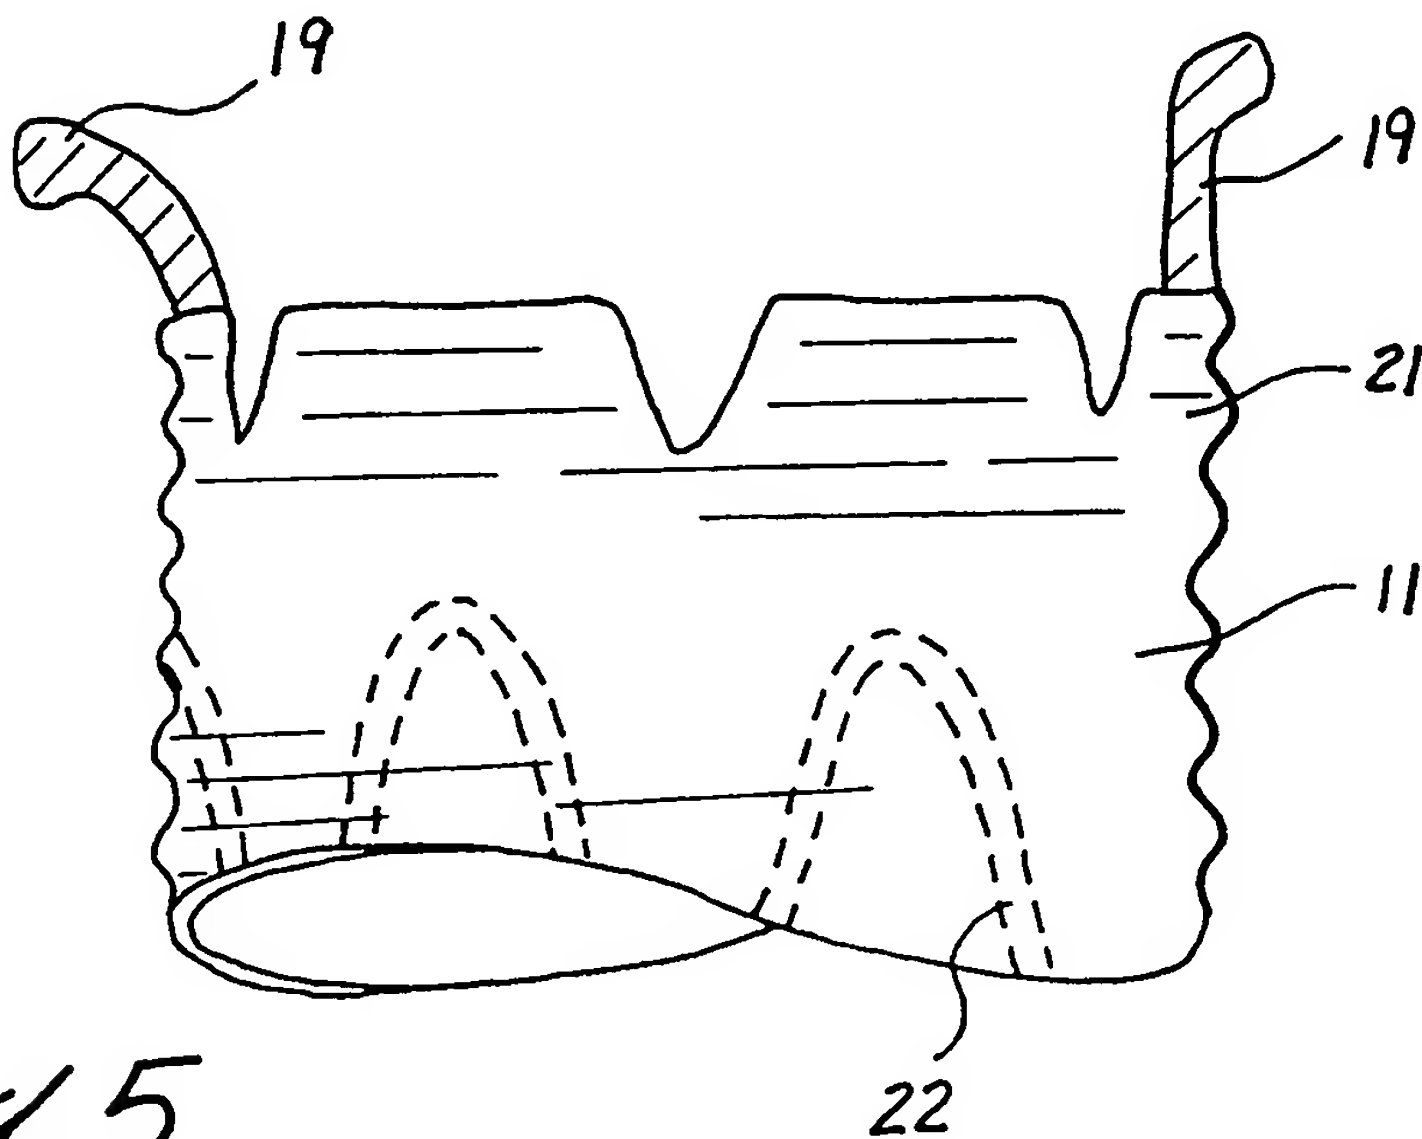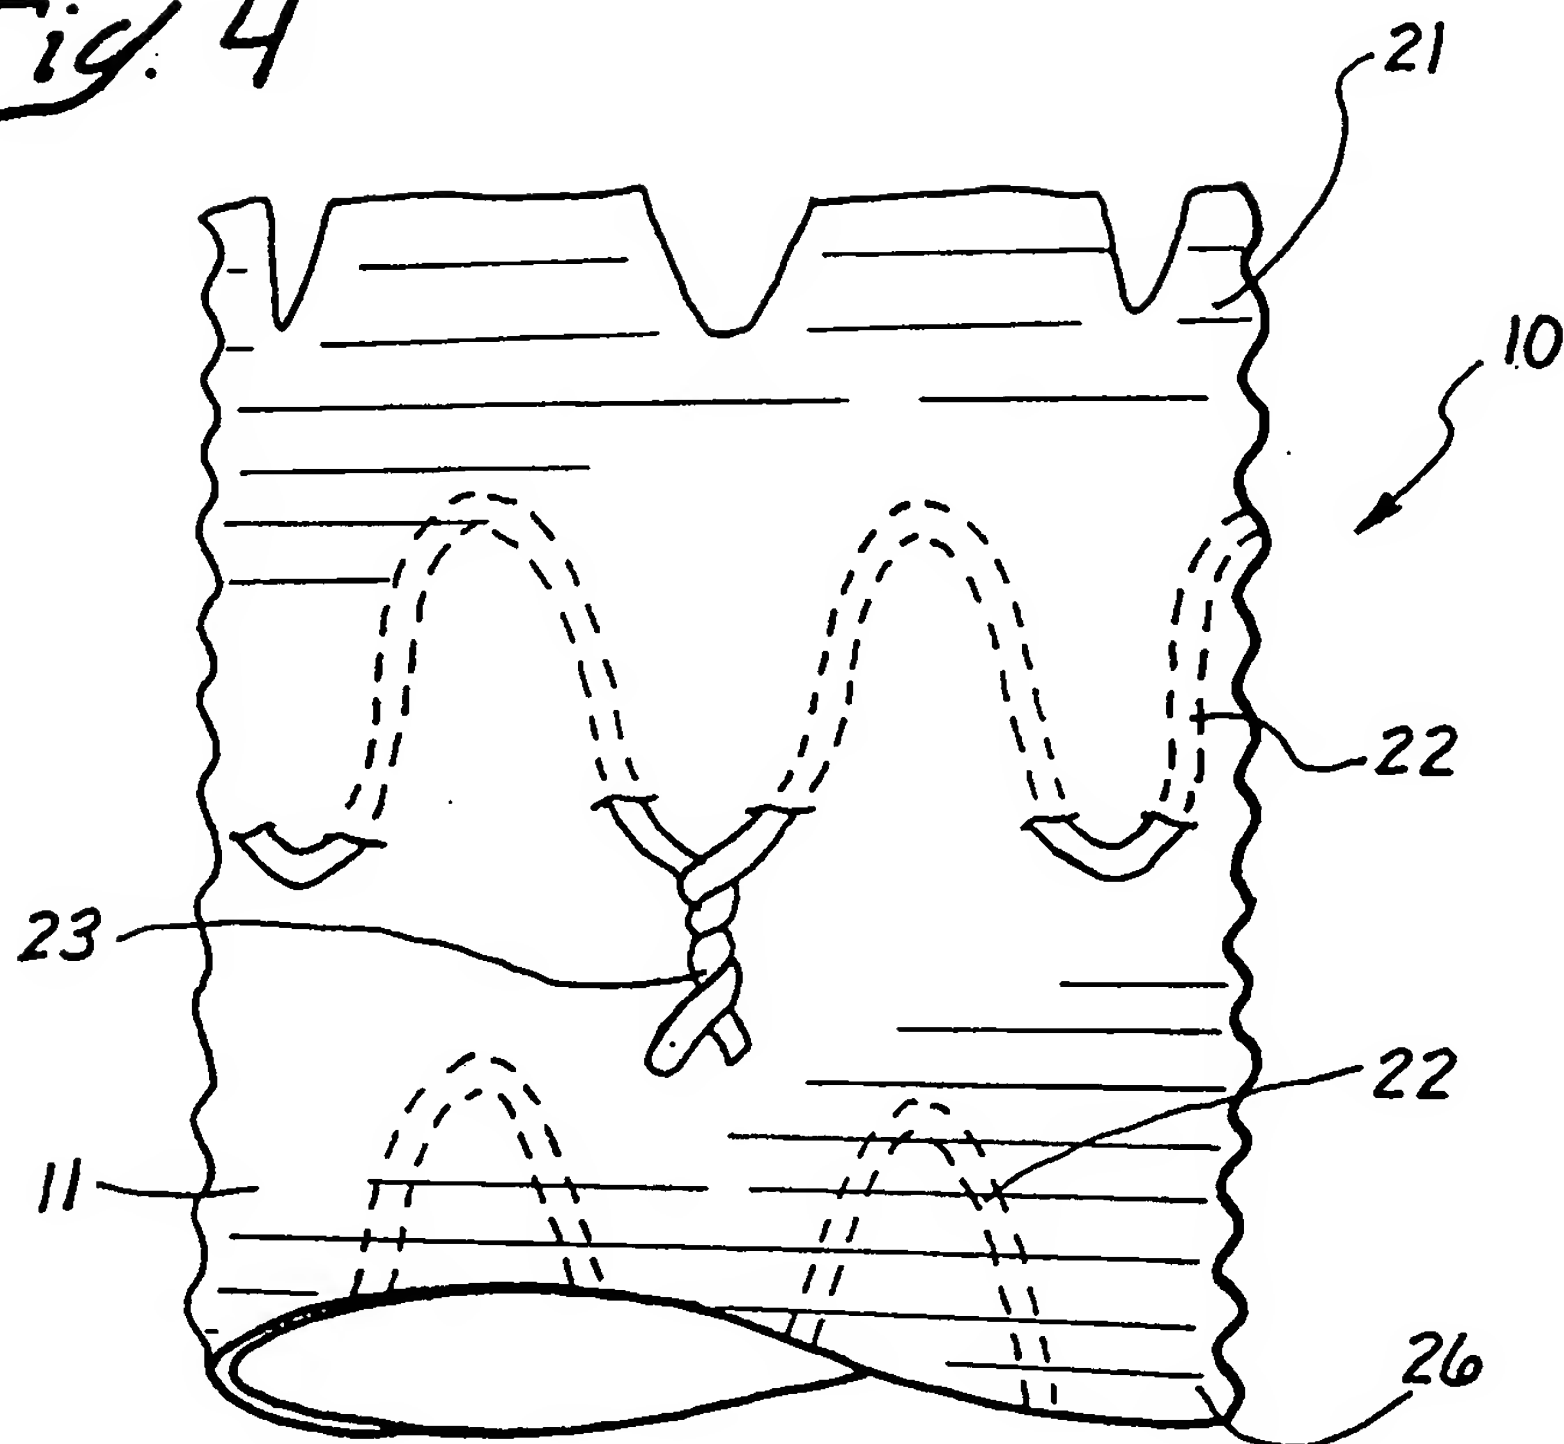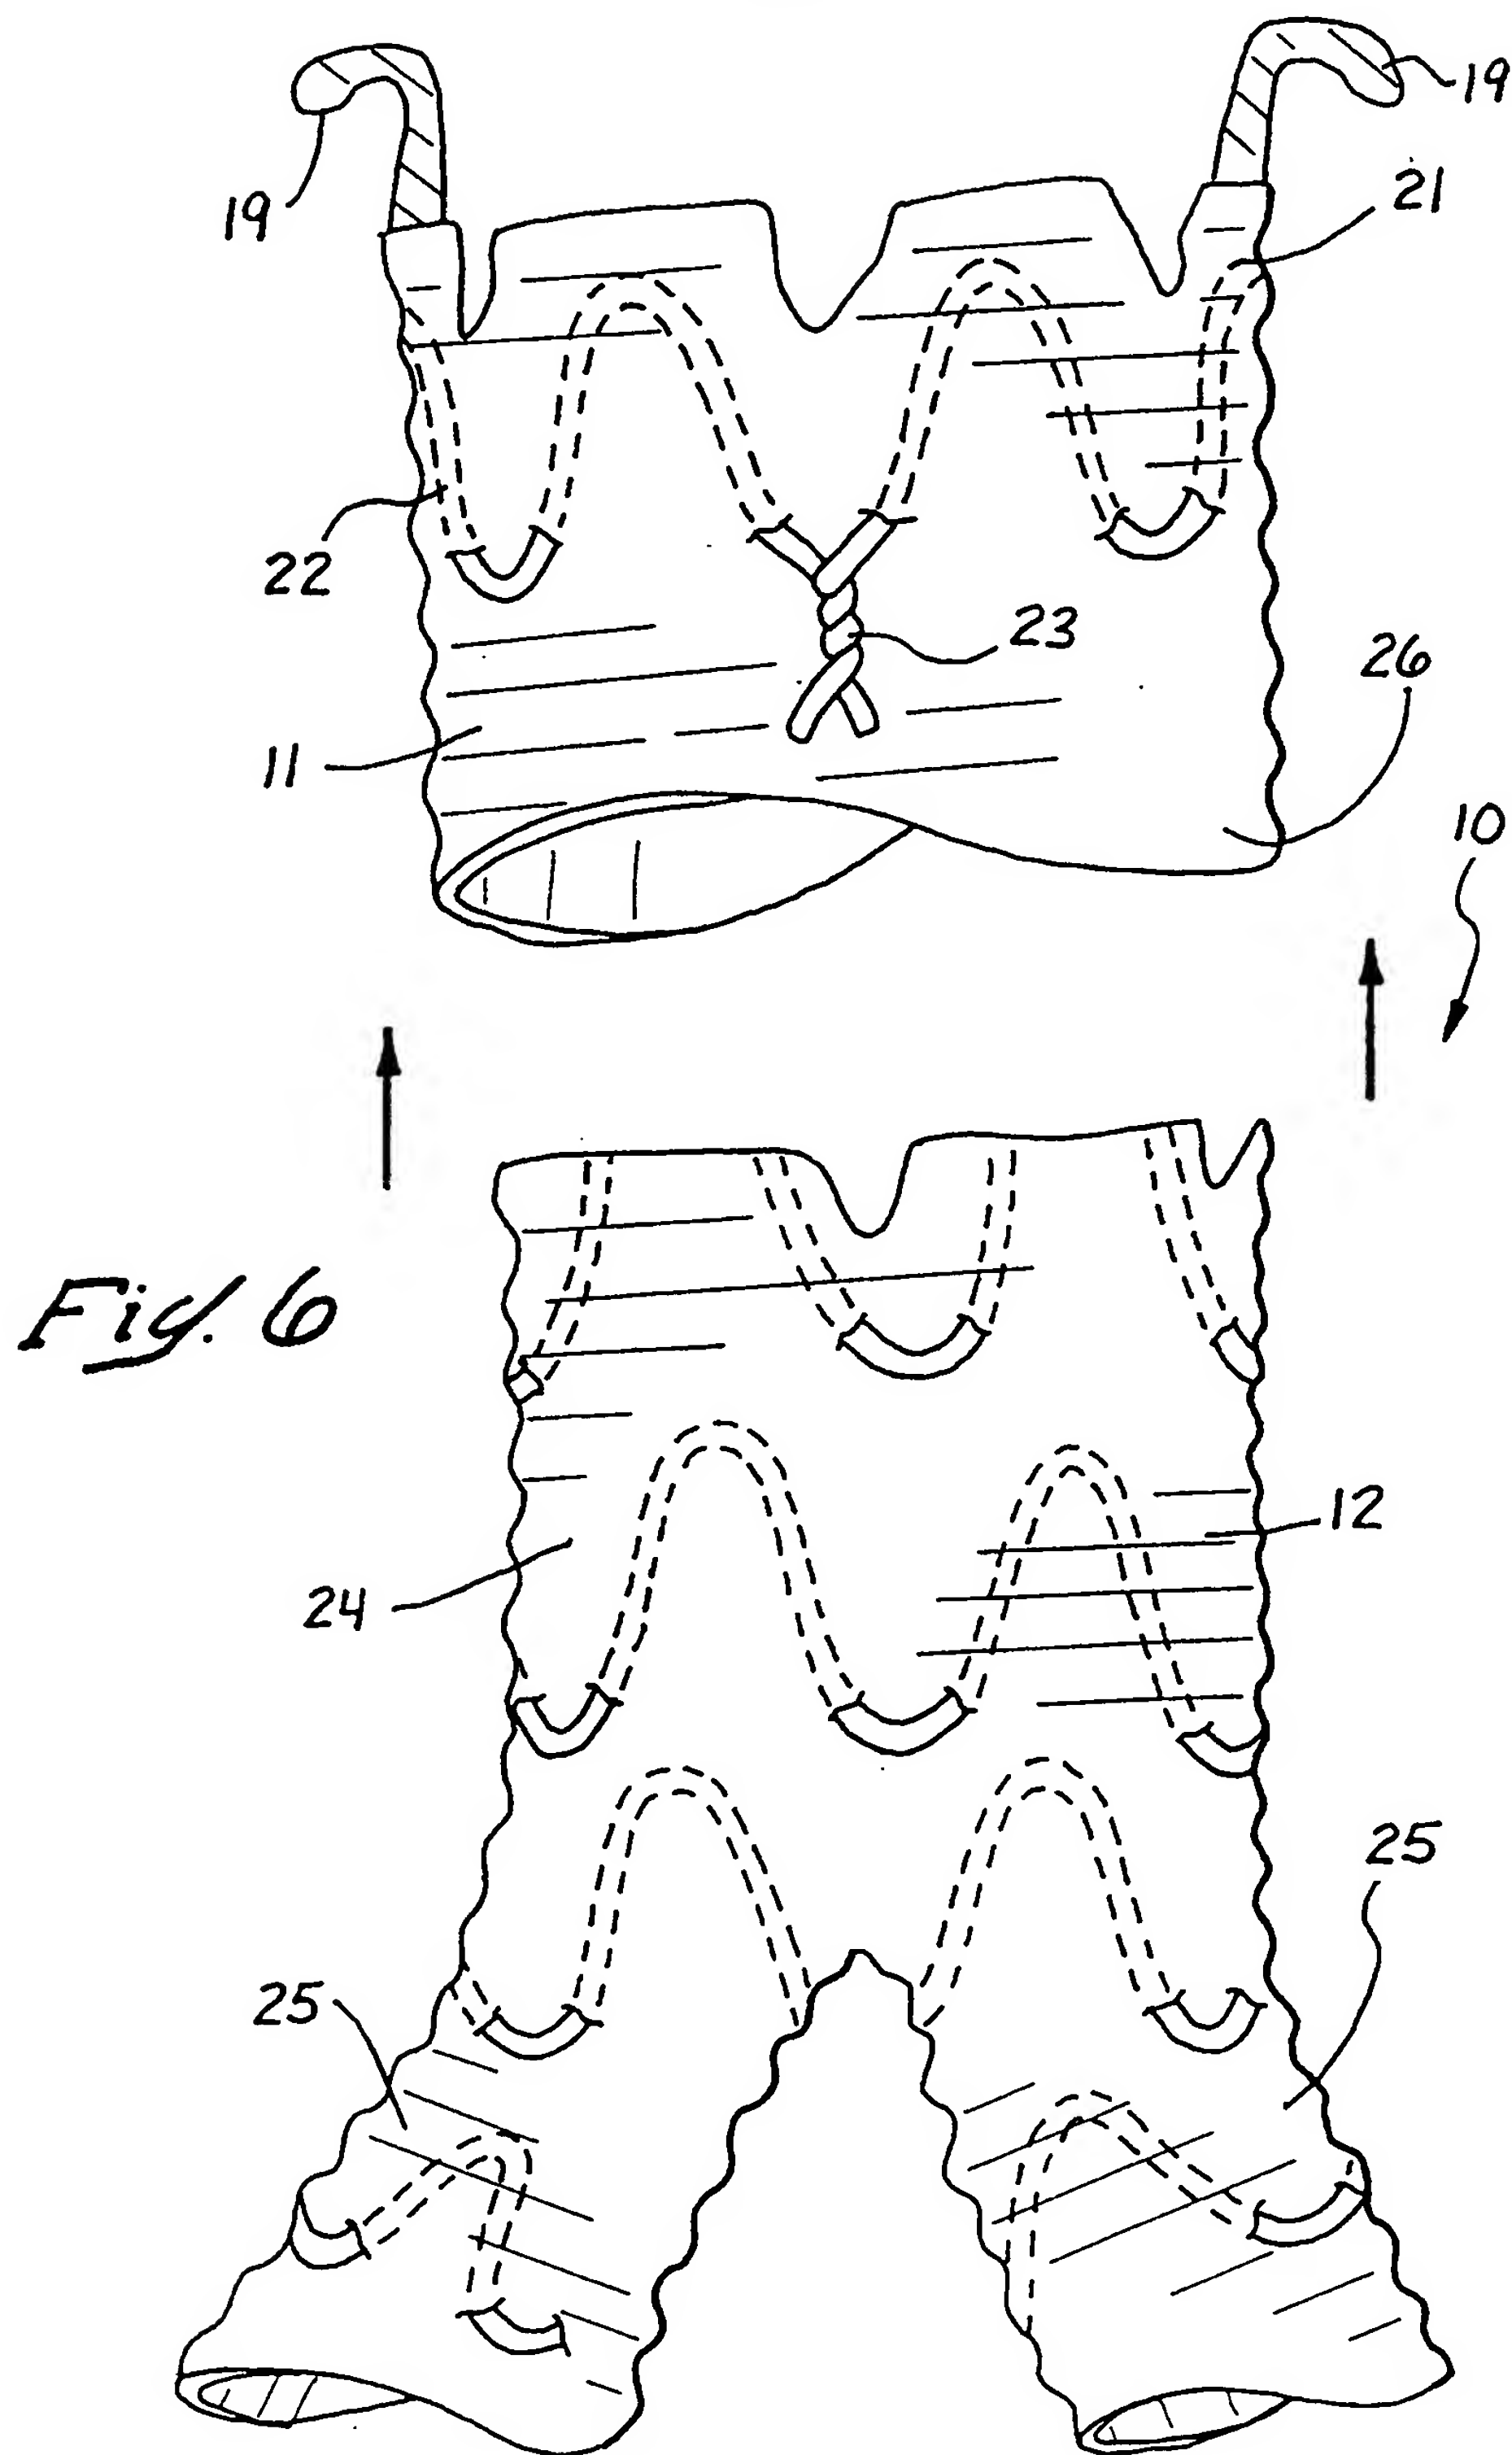


5/8

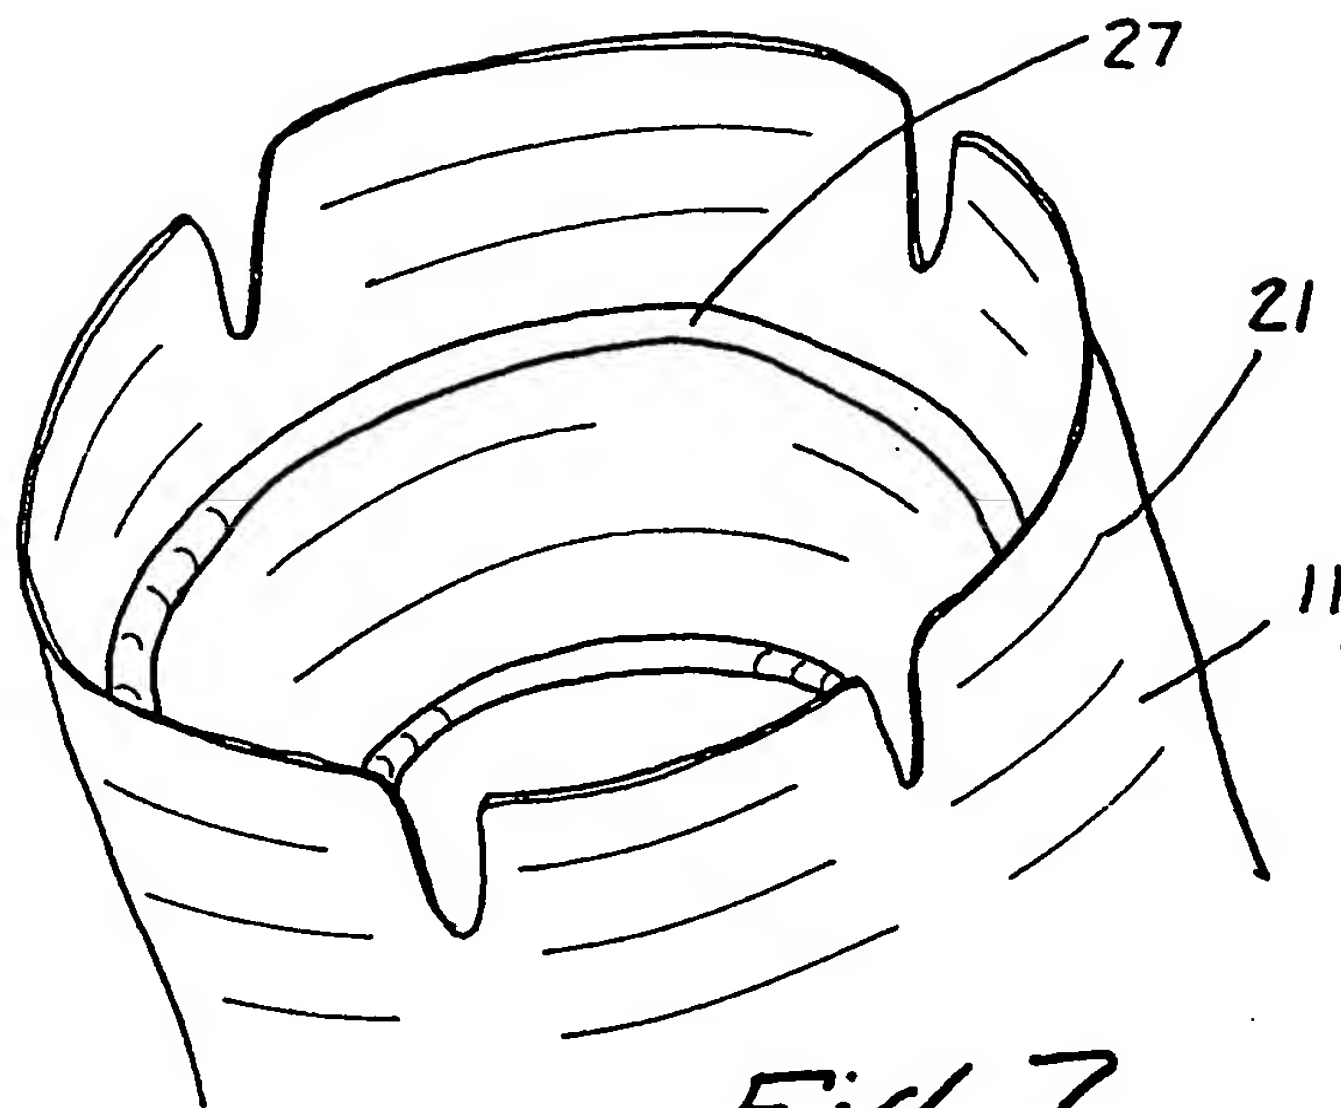

*Fig. 7*

*Fig. 13*

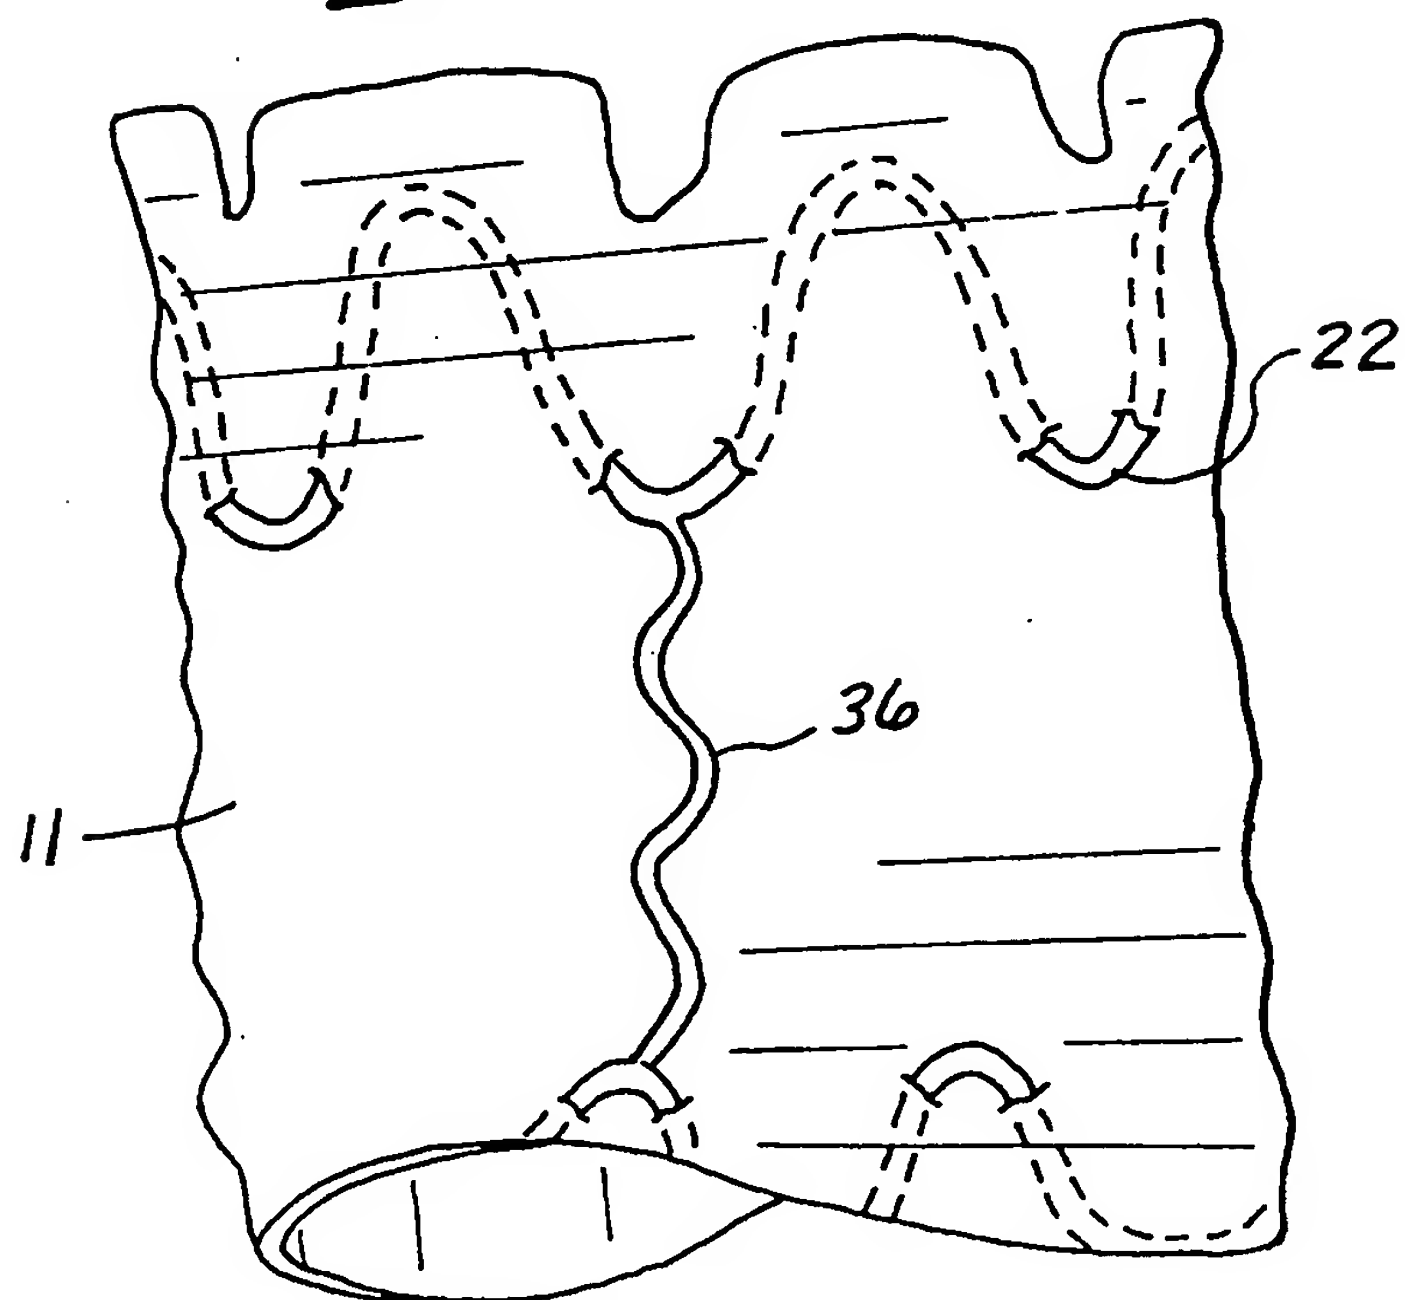



6/8

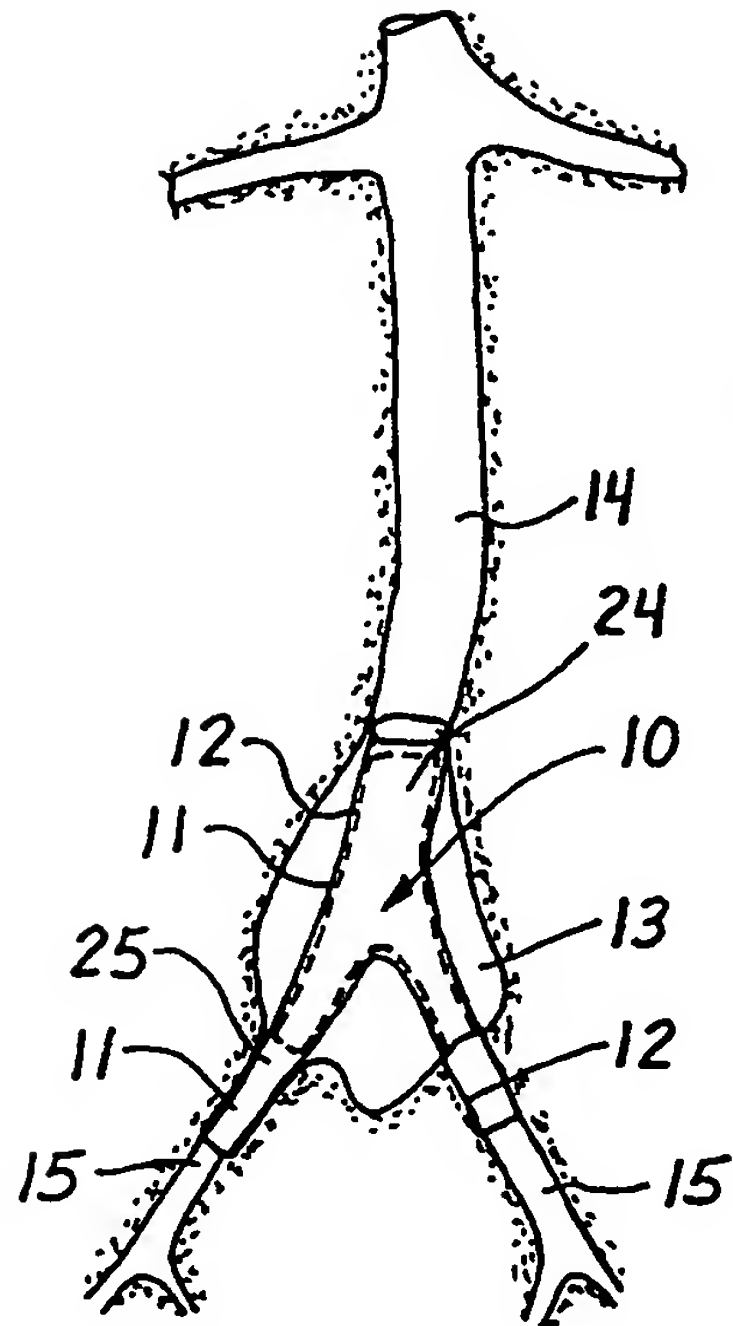


Fig. 8

Fig. 9

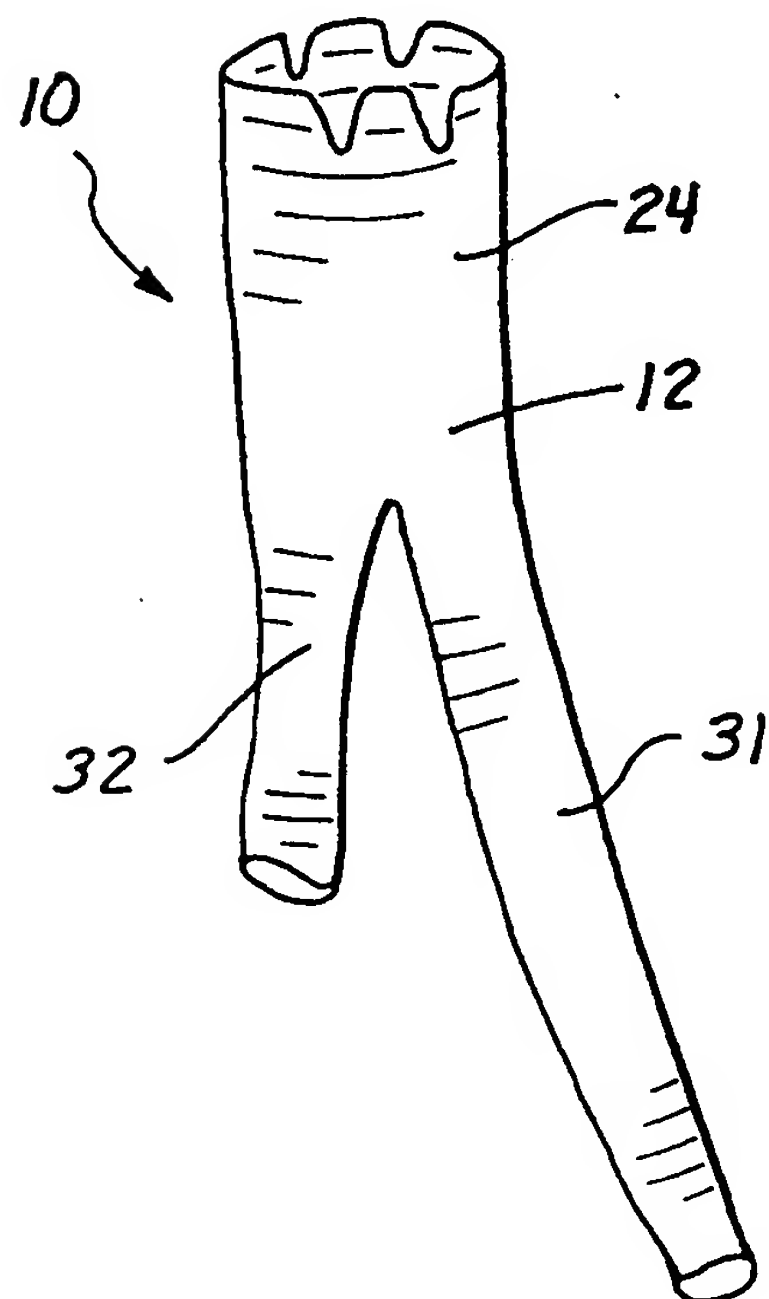
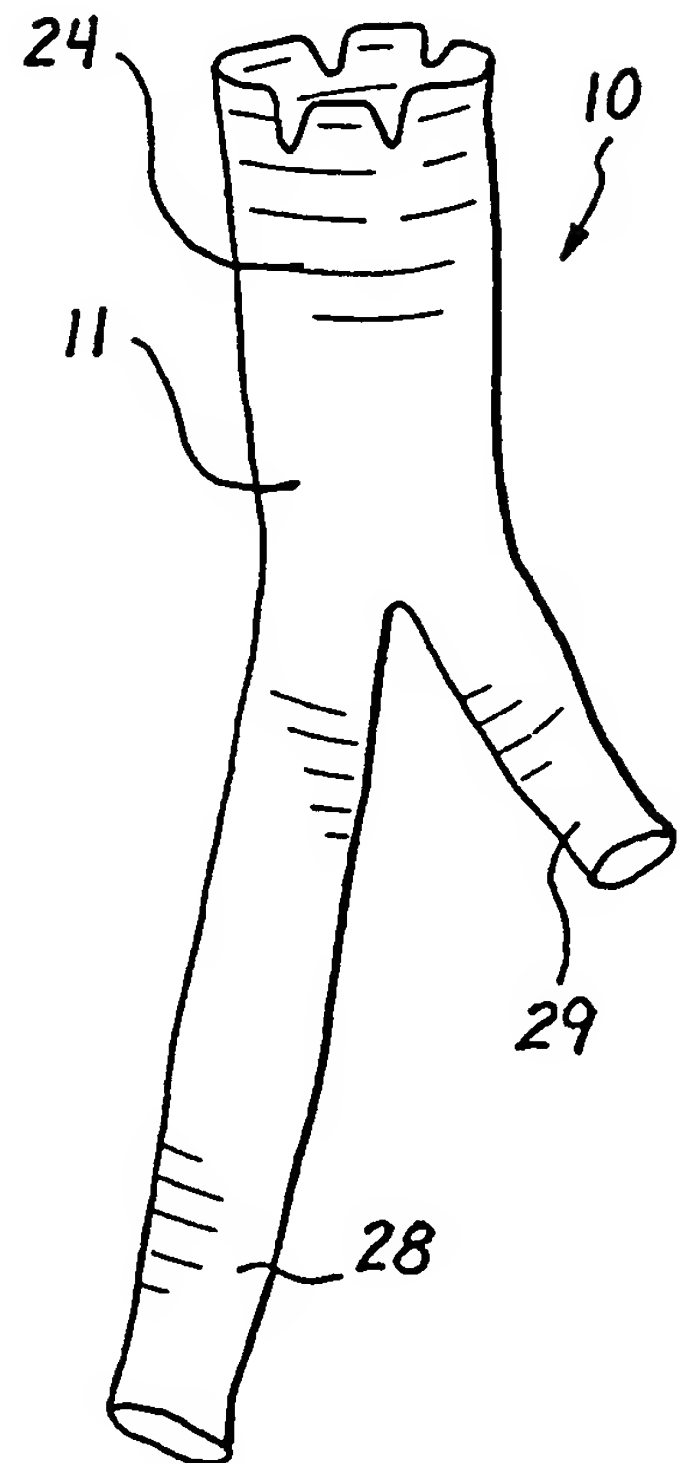


Fig. 10

7/8



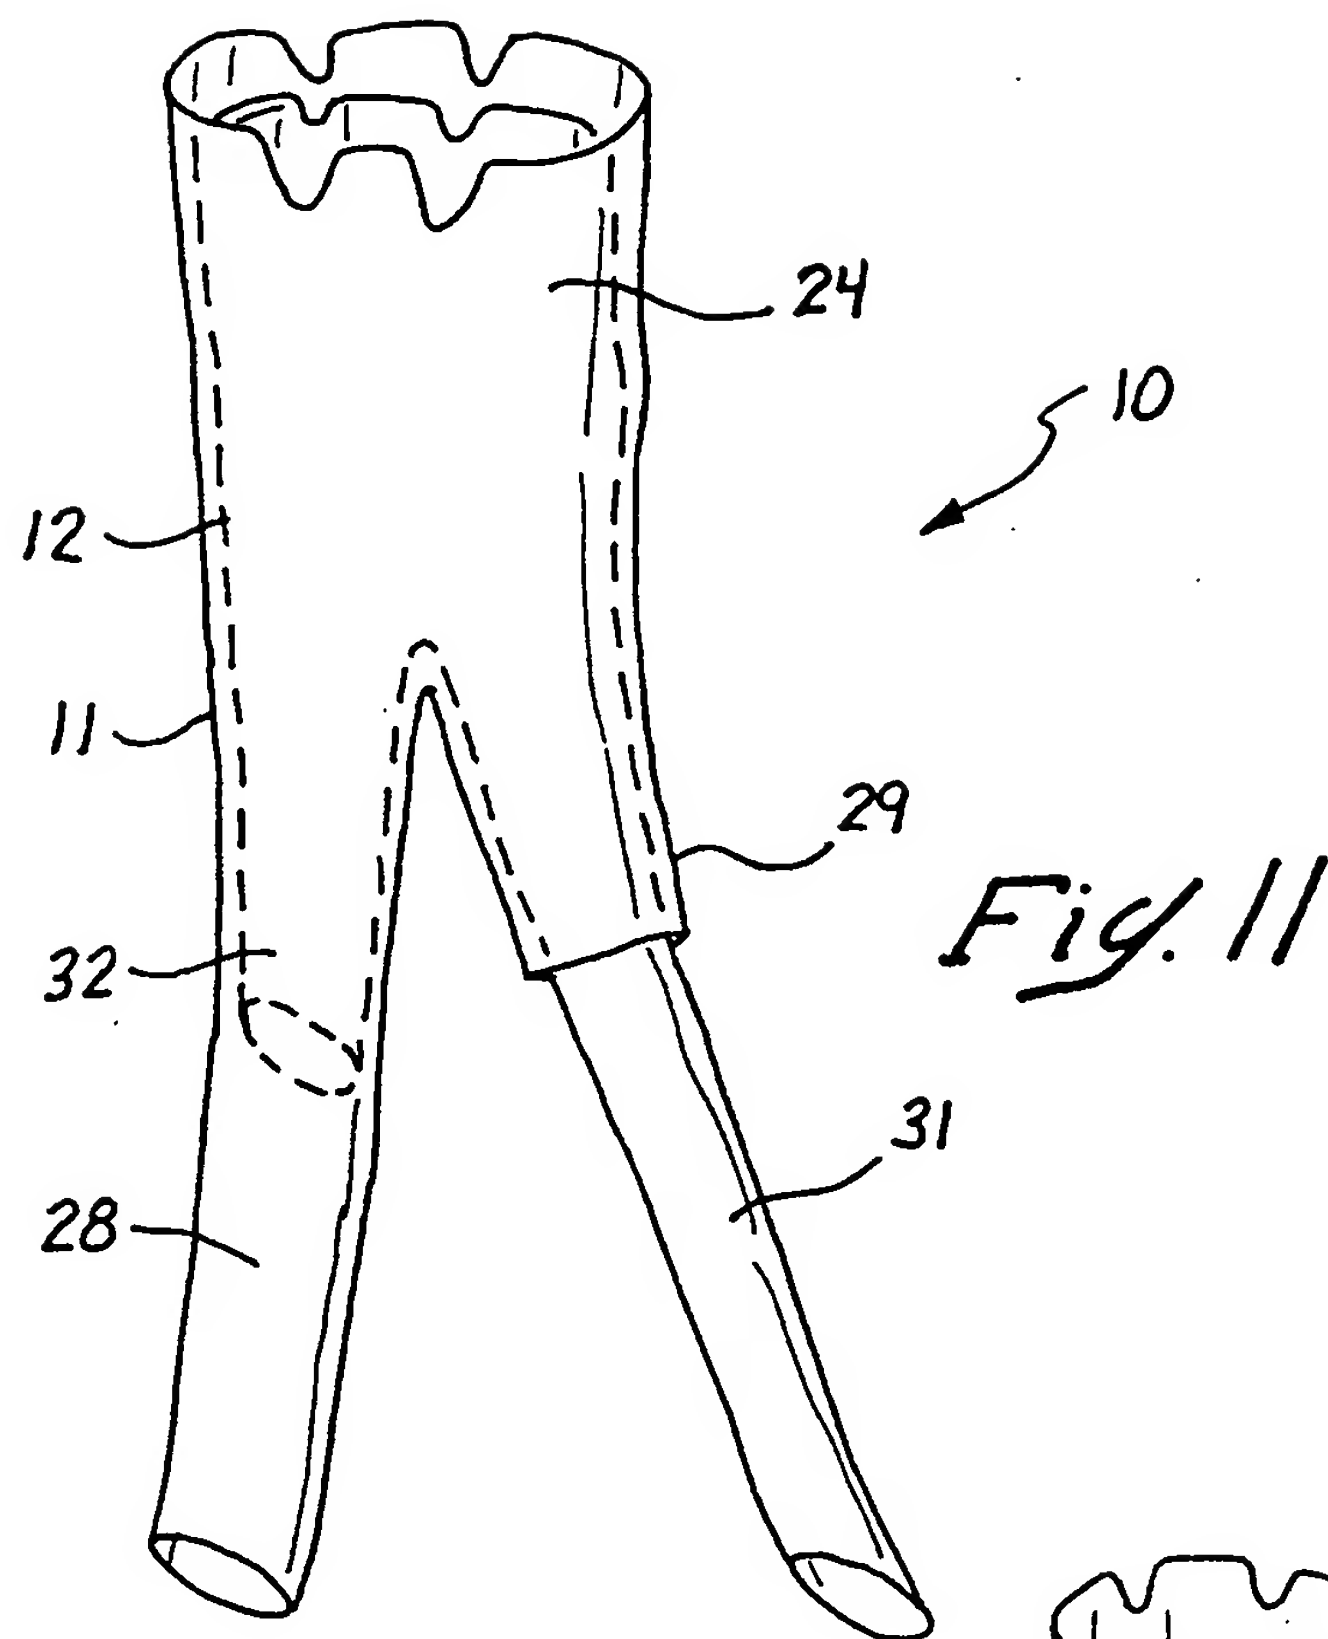


Fig. 12

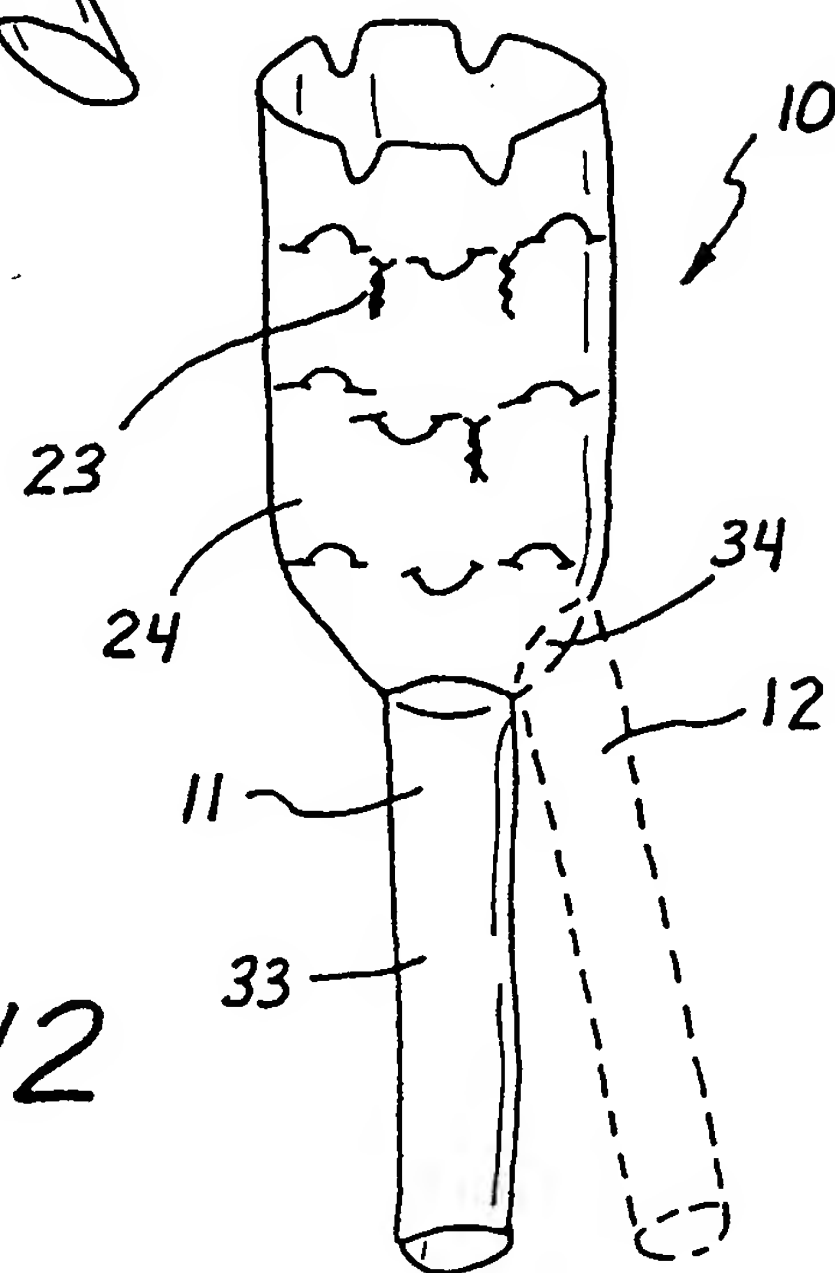

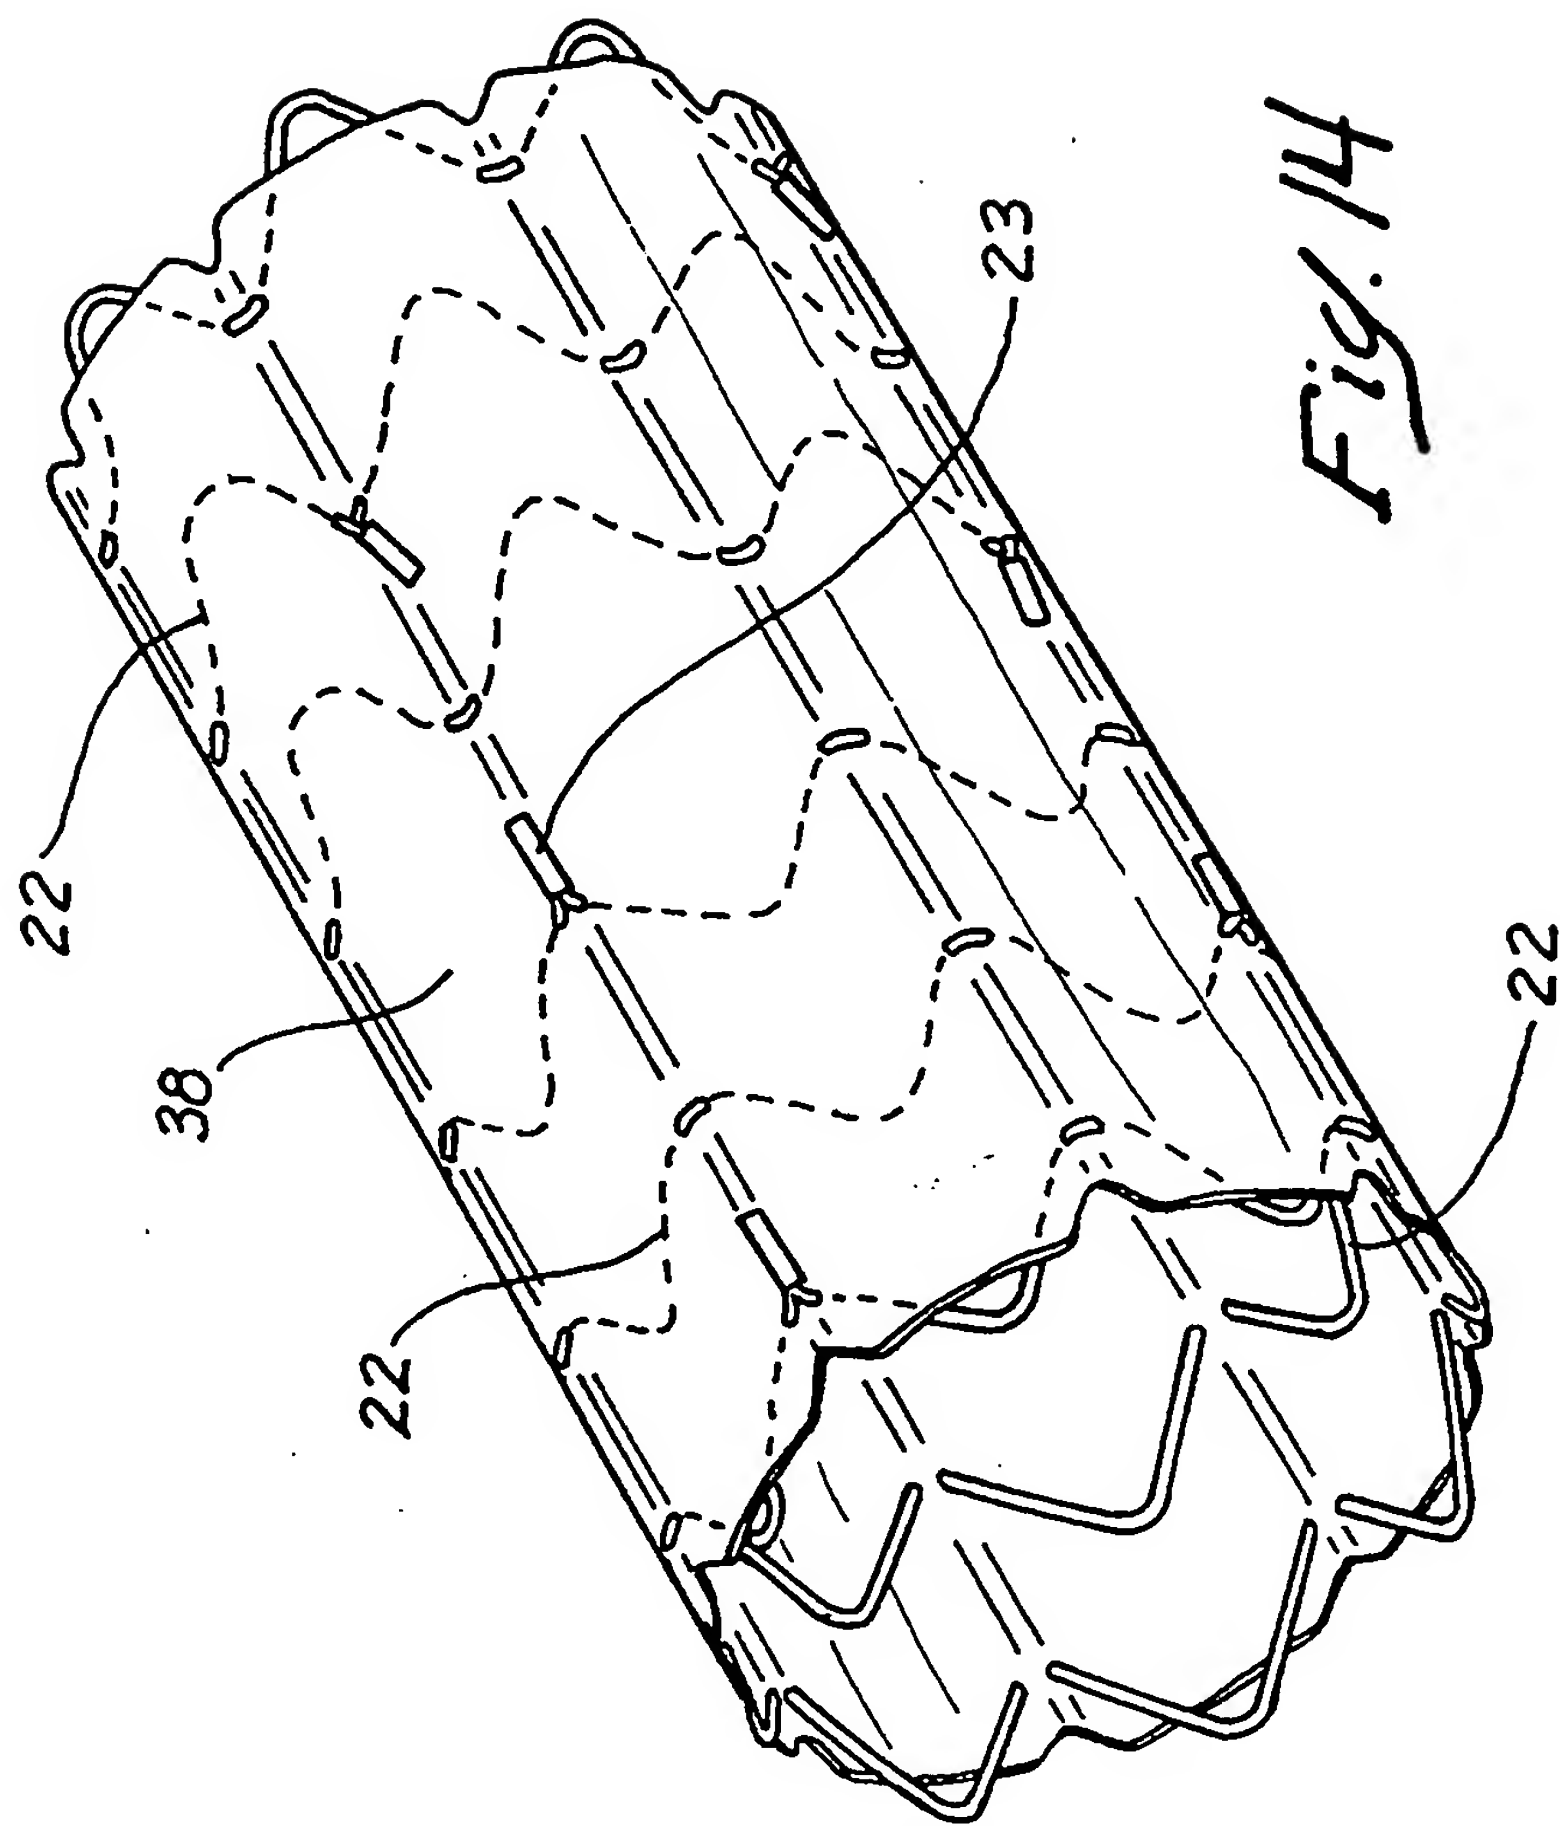

## INTERNATIONAL SEARCH REPORT

Internat Application No

PCT/US 00/16457

A. CLASSIFICATION OF SUBJECT MATTER  
IPC 7 A61F2/06

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 843 160 A (RHODES VALENTINE J) 1 December 1998 (1998-12-01) figures 1-4,8-10 column 7, line 35 - line 50 column 8, line 24 - line 46 column 13, line 52 -column 15, line 21	1,2
A	---	14,18,20
X	US 5 662 675 A (POLANSKYJ STOCKERT ODARKA ET AL) 2 September 1997 (1997-09-02) figures 1,2,4-8 column 7, line 8 - line 31 column 8, line 35 - line 67 column 10, line 47 -column 11, line 3	1,2,20
A	---	14,18
	--- -/--	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

## \* Special categories of cited documents :

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*&\* document member of the same patent family

Date of the actual completion of the international search

9 October 2000

Date of mailing of the international search report

19/10/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Mary, C

## INTERNATIONAL SEARCH REPORT

Internal Application No  
PCT/US 00/16457

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
P, X	US 6 010 529 A (KARWOSKI THEODORE ET AL) 4 January 2000 (2000-01-04) figures 1A-2D claims 10-27	14
A	---	1, 2, 18, 20
P, X	US 6 045 557 A (YU WEIYUN ET AL) 4 April 2000 (2000-04-04) figures 2-4, 8 column 5, line 37 -column 6, line 6	1, 2, 18, 20
A	---	14
E	WO 00 45742 A (BARD INC C R) 10 August 2000 (2000-08-10) figures 1, 2 claim 1	14, 20
A	---	1, 2, 18
E	WO 00 38590 A (BARKER STEPHEN GEORGE EDWARD) 6 July 2000 (2000-07-06) page 4, line 10 -page 5, line 14 figures 1, 2	14
A	-----	1, 2, 18, 20

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. Claims: 1,2

A double-grafts endovascular prosthesis with overlapping part.

2. Claim : 14

An intraluminal graft composed of two layers of a material and a plurality of wires sandwiched between said layers.

3. Claim : 18

A tubular graft reinforced along its length by a plurality of wires which are woven throughout the fabric of the graft.

4. Claim : 20

An intraluminal graft reinforced with a plurality of wires wherein at least one end of the graft is provided with a wire which has alternate apices extending beyond at least said end to extent across the lumen of a second vessel opening into the first vessel in which the graft is being placed without occluding that lumen.



# INTERNATIONAL SEARCH REPORT

Information on patent family members

Internal

Application No

PCT/US 00/16457

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 5843160	A	01-12-1998	NONE	
US 5662675	A	02-09-1997	NONE	
US 6010529	A	04-01-2000	AU 5898498 A EP 0971643 A WO 9826731 A	15-07-1998 19-01-2000 25-06-1998
US 6045557	A	04-04-2000	AU 7486296 A AU 706084 B AU 7486396 A AU 7486496 A WO 9717910 A WO 9717911 A WO 9718006 A BR 9611371 A BR 9611441 A CA 2236602 A CN 1207658 A CN 1207659 A EP 0955952 A EP 0955953 A JP 2000500046 T JP 2000500047 T US 6099558 A	05-06-1997 10-06-1999 05-06-1997 05-06-1997 22-05-1997 22-05-1997 22-05-1997 28-12-1999 28-12-1999 22-05-1997 10-02-1999 10-02-1999 17-11-1999 17-11-1999 11-01-2000 11-01-2000 08-08-2000
WO 0045742	A	10-08-2000	WO 0045741 A WO 0045743 A	10-08-2000 10-08-2000
WO 0038590	A	06-07-2000	GB 2346559 A	16-08-2000

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**